


Mass Spectrum

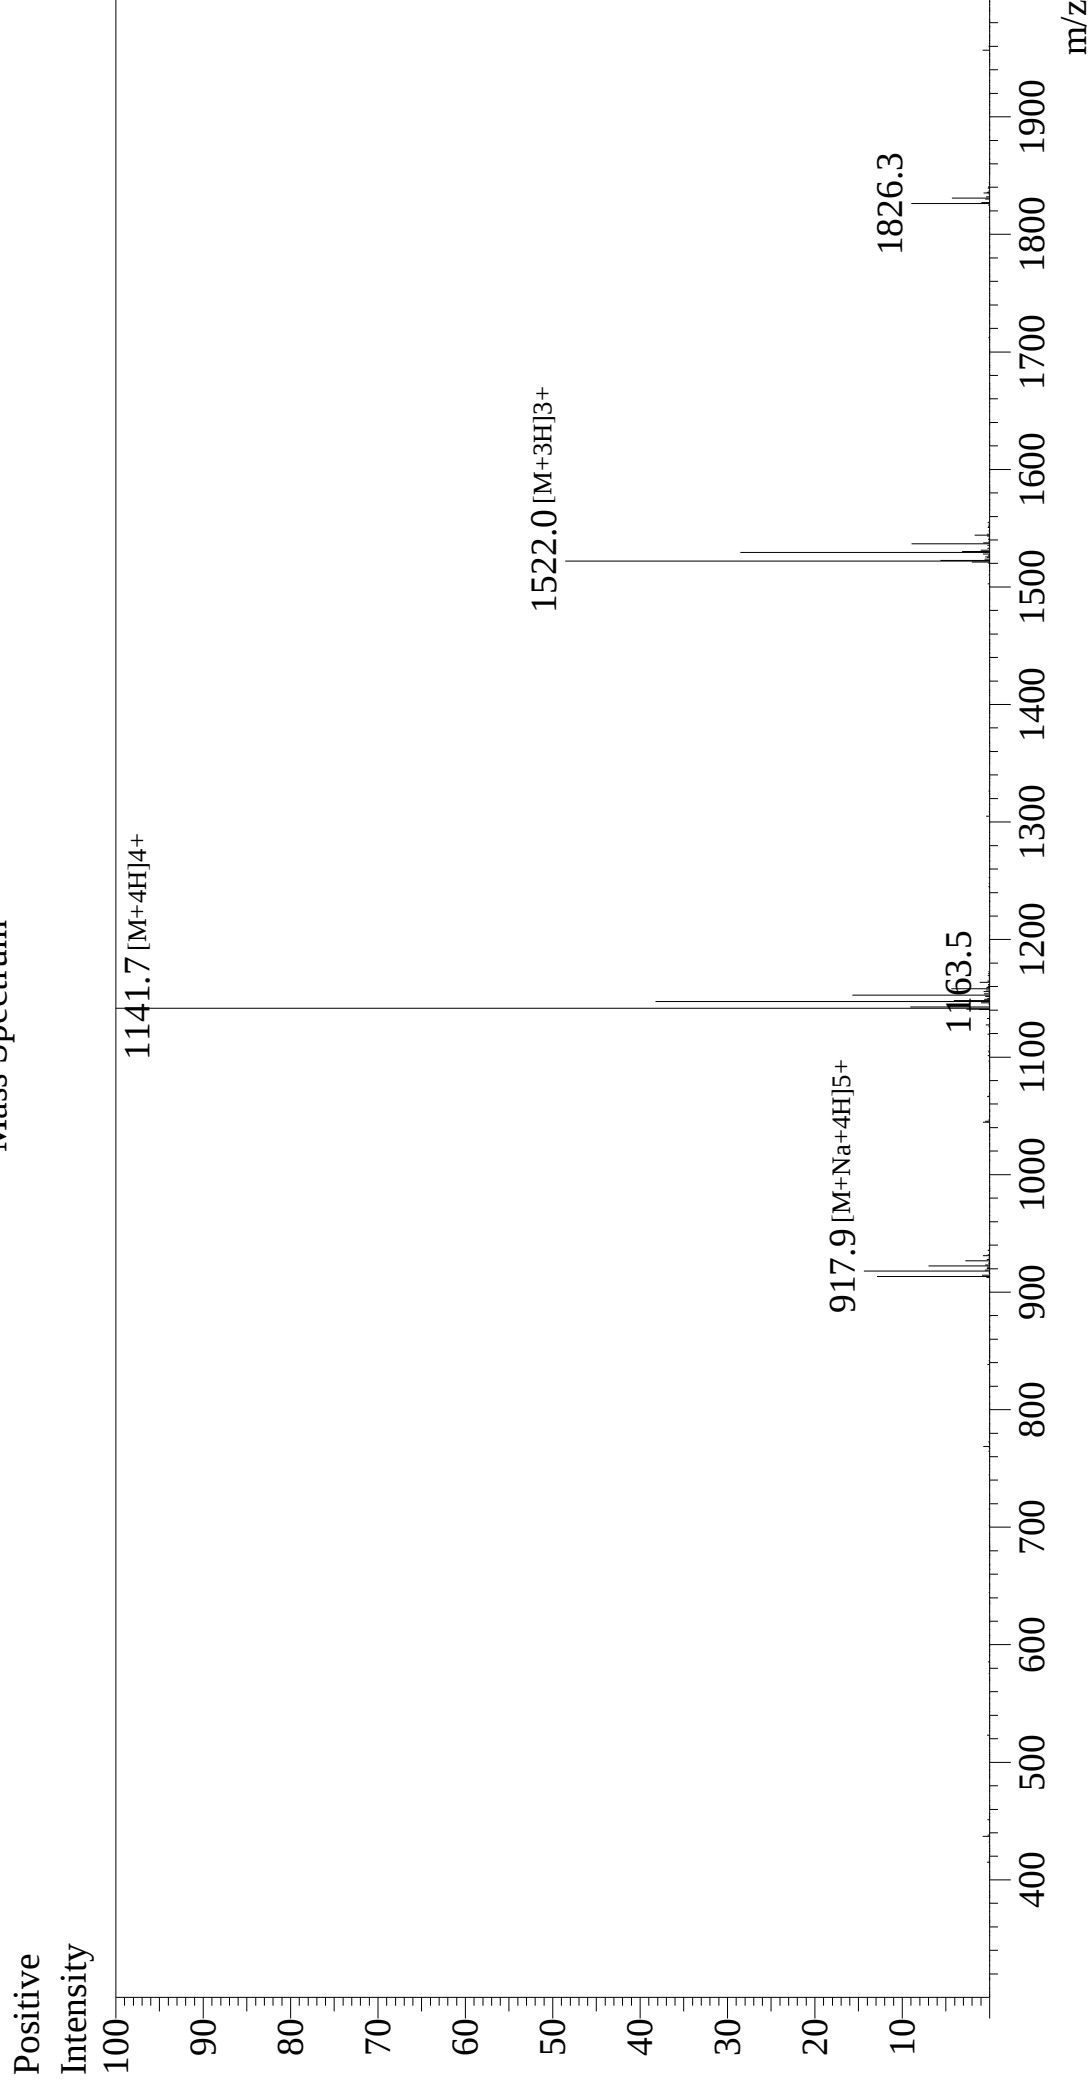

Sample Information

Month-Day Processed : 09/05/25
 Time Processed : 12:59:32
 Injection Volume : 0.4
 Sample Name : [D-ALA]19-Mazdutide
 Cat No. : RP30908
 Lot No. : E9766125HC
 Theoretical MW : 4563.14
 Observed MW : 4562.8

Interface : ESI

Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H₂O/50%MeOH

Equipment : ZJ21010035