


Mass Spectrum

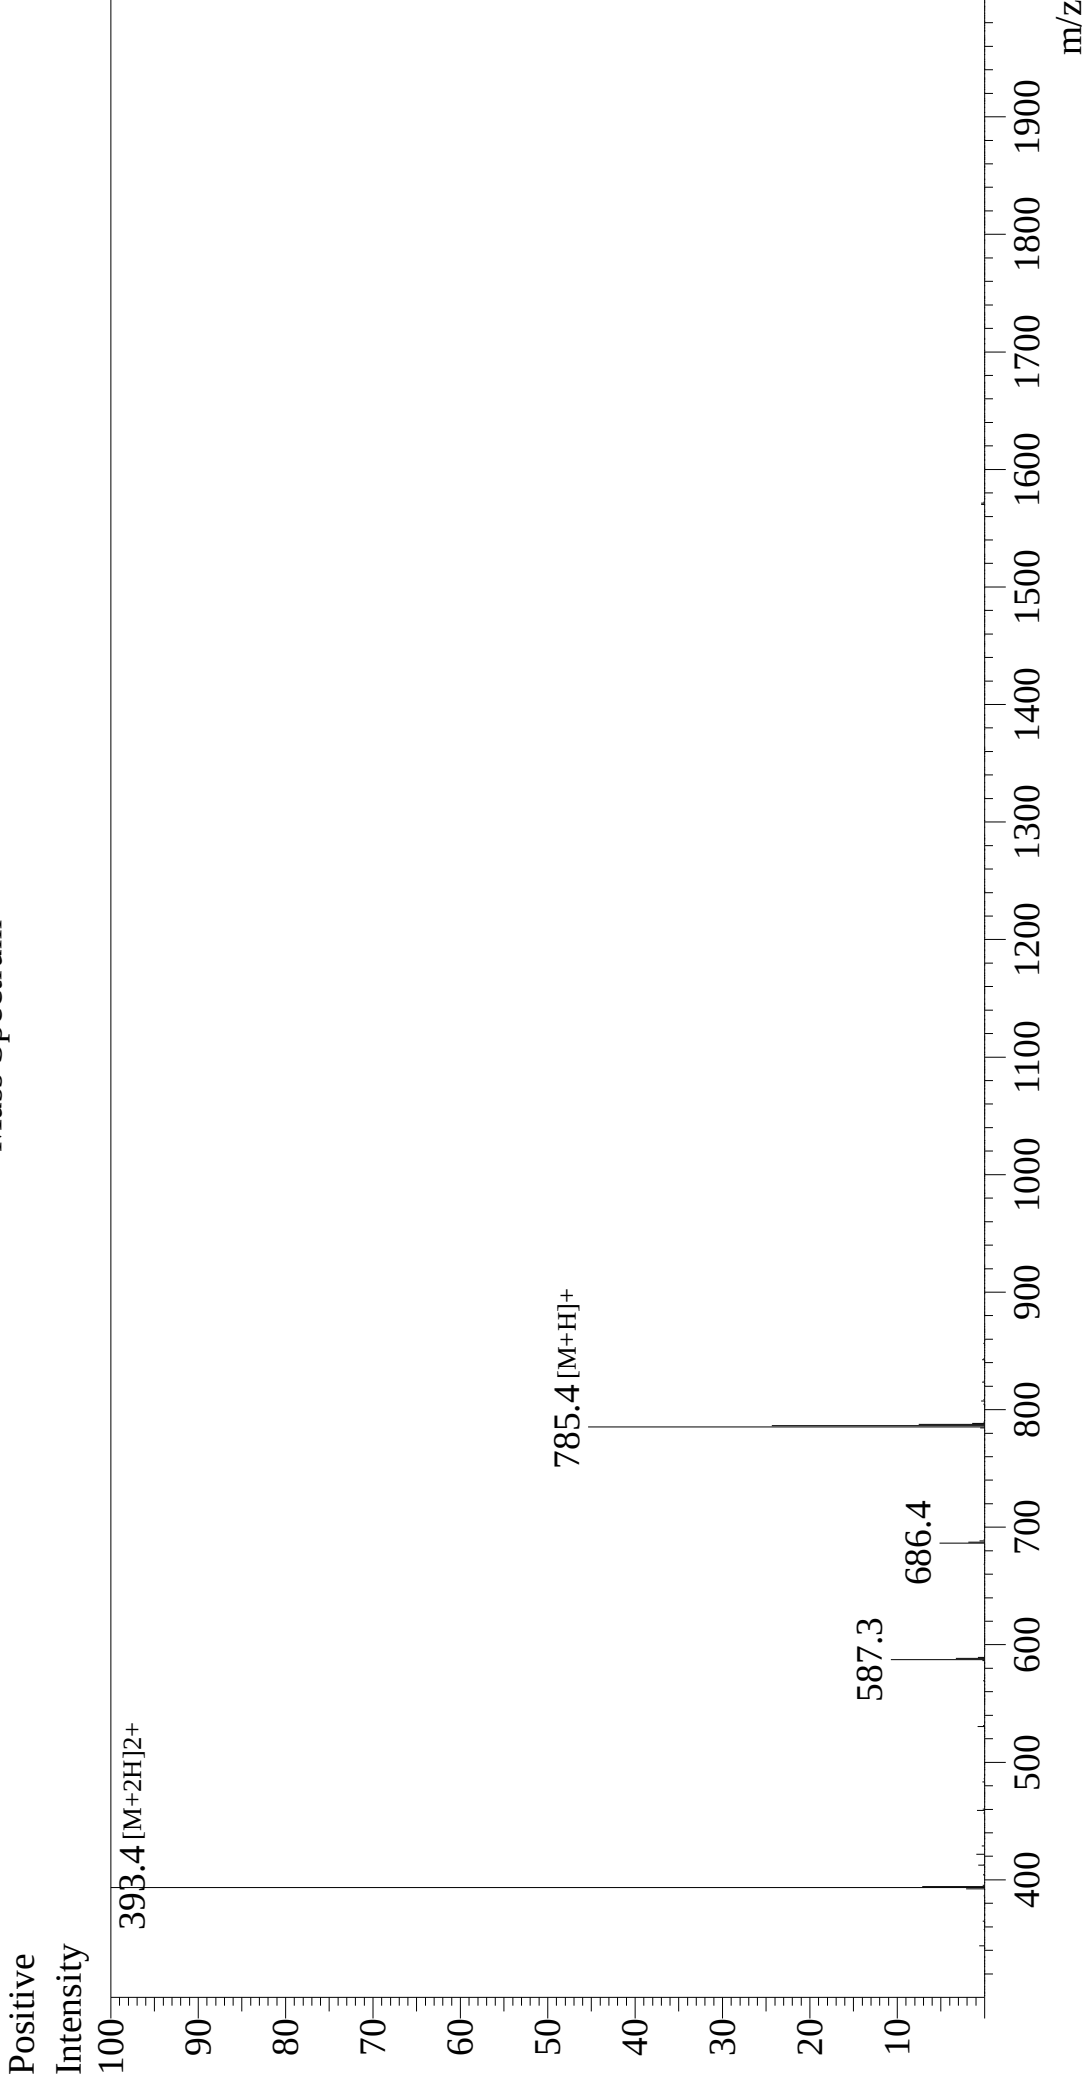

Sample Information
Month-Day Processed : 04/17/26
Time Processed : 8:52:30
Injection Volume : 0.3
Sample Name : KRAS G12V Peptide (VVGAVGVGK)
Cat No. : RP30228
Lot No. : E9772326D
Theoretical MW: 784.95
Observed MW : 784.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200
Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH