

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
Cat No. : RP11095
Lot No. : E9853922B
Time Processed : 8:04:55 AM
Month-Day-Year Processed : 03/10/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow: 1 ml/min
Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ19010141

<Chromatogram>

mV

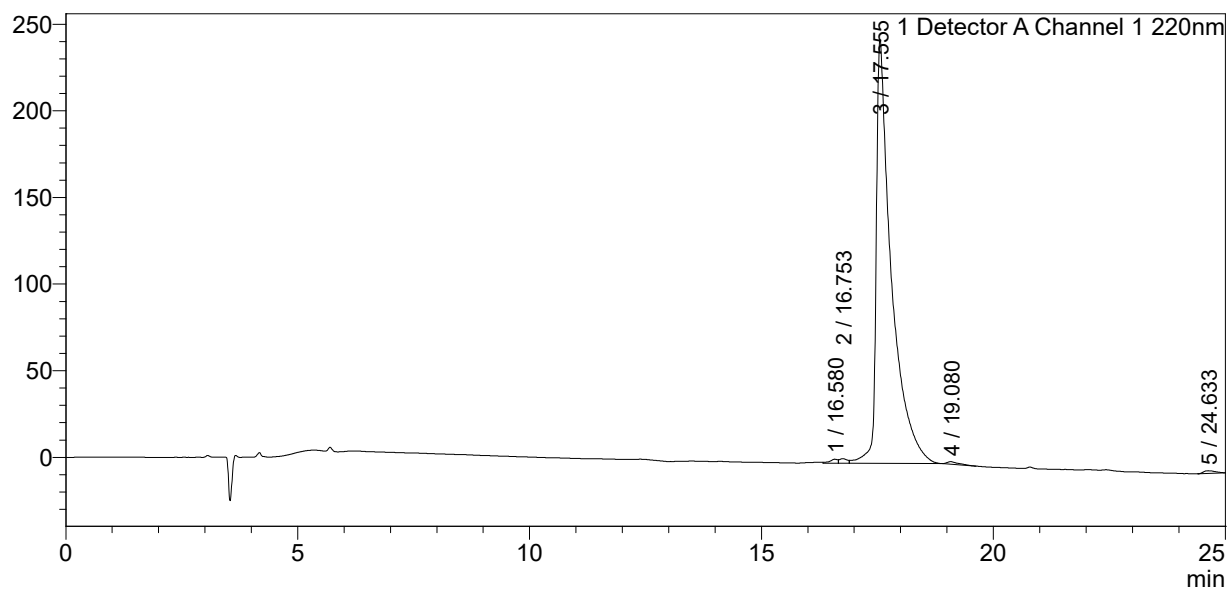

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.580	26783	2280	0.471
2	16.753	30521	2645	0.537
3	17.555	5574981	244616	98.005
4	19.080	26756	1521	0.470
5	24.633	29418	1593	0.517
Total		5688459	252653	100.000