

Sample Name : Substance P
 Cat No. : RP10178
 Lot No. : E9962124K
 Time Processed : 16:13:40
 Month-Day-Year Processed : 11/12/2024
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ23010112

<Chromatogram>

mV

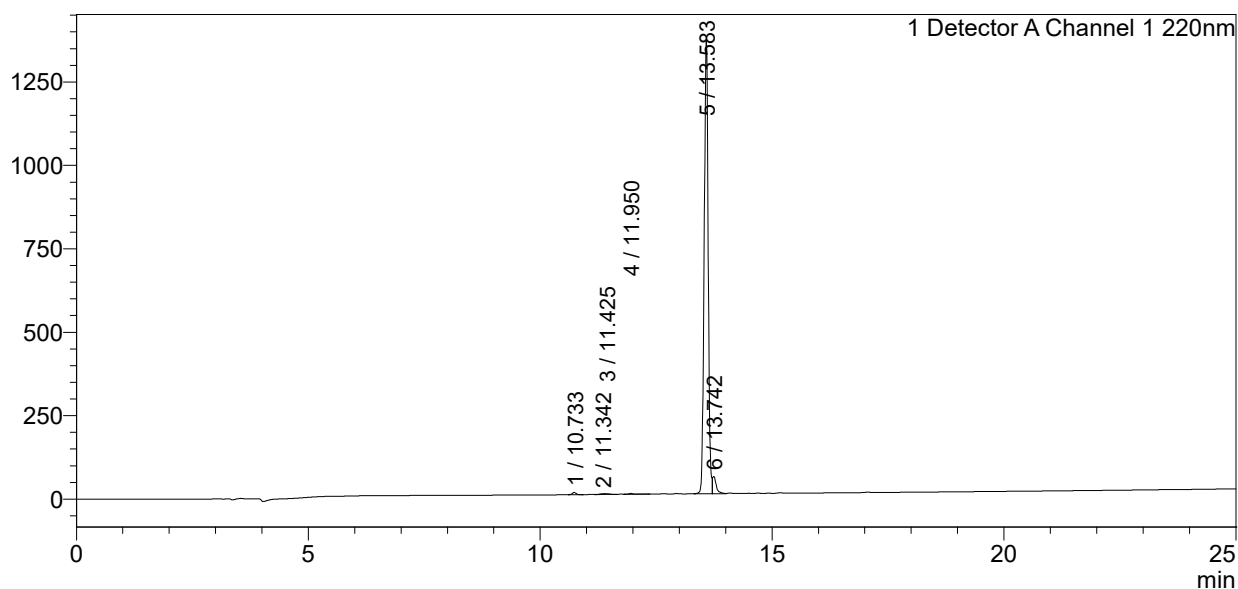

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.733	40888	6721	0.474
2	11.342	18992	2562	0.220
3	11.425	21134	2743	0.245
4	11.950	31893	2589	0.369
5	13.583	8218253	1358941	95.186
6	13.742	302697	51462	3.506
Total		8633857	1425018	100.000