


Mass Spectrum

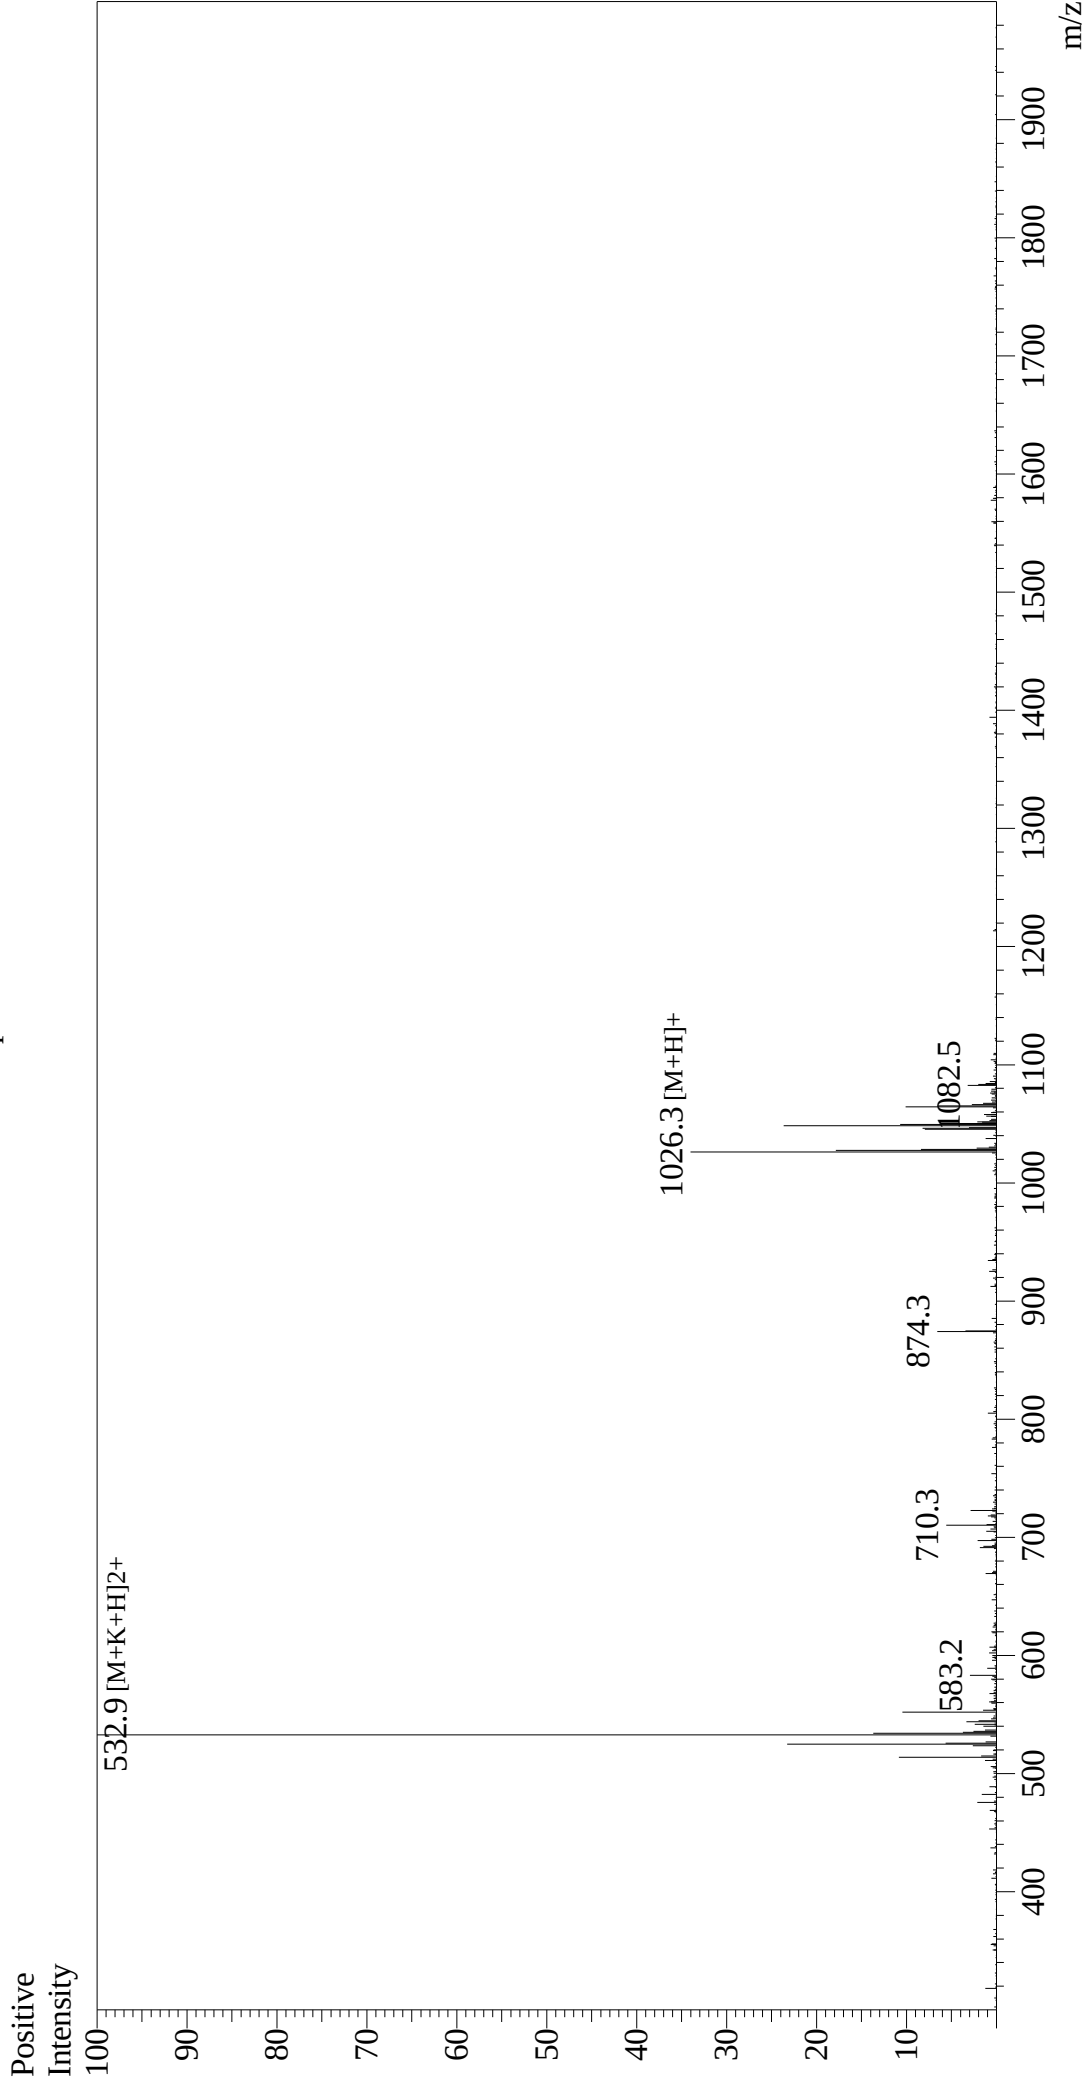

Sample Information

Month-Day Processed :	02/13/23	Equipment	: ZJ21010035
Time Processed :	18:22:00	Interface Bias	: +4.5 kV
Injection Volume :	0.2	Drying Gas Flow	: 5 L/min
Sample Name :	Influenza A NP(366-374) Strain A/PR/8/35	T.Flow	: 0.2 ml/min
Cat No. :	RP20267	B.conc	: 50% H ₂ O/50% MeOH
Lot No. :	E9976823B		
Theoretical MW :	1026.12		
Observed MW :	1026.8		