

Sample Name :AMARA peptide
 Cat. No. : RP20472
 Lot. No. : PE8991902
 Time Processed : 9:29:32
 Month-Day-Year Processed : 03/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	70	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	10	
40.00	Pumps	Pump A B.Conc	10	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

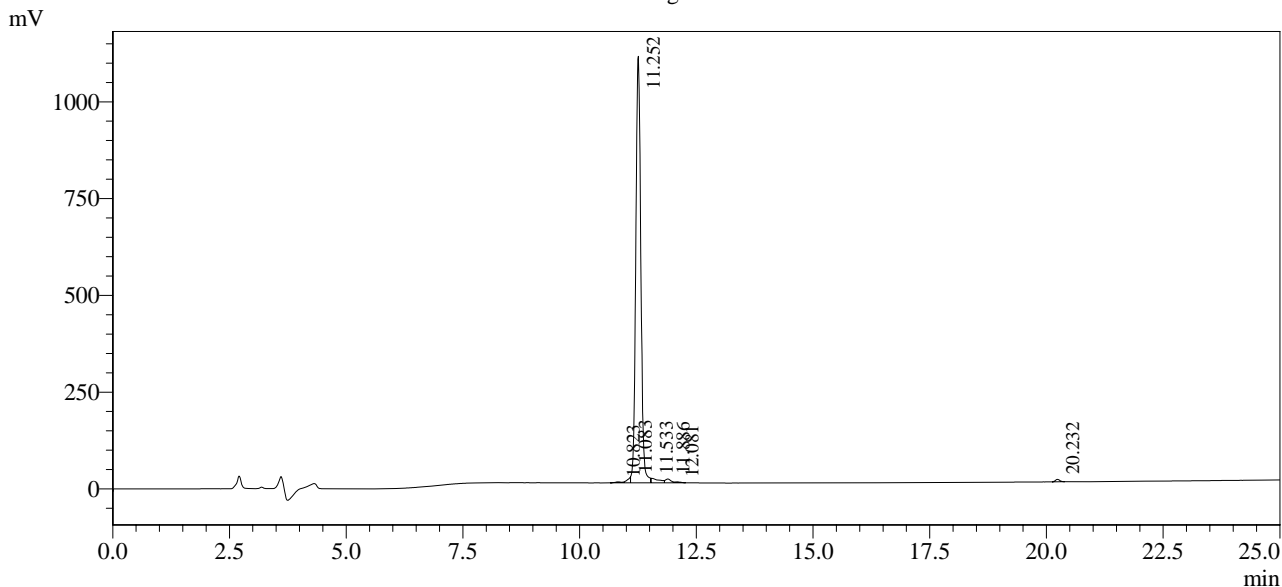

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.823	23376	2484	0.270
2	11.083	69565	14025	0.805
3	11.252	8279039	1101928	95.756
4	11.533	137007	11616	1.585
5	11.886	78548	9716	0.908
6	12.081	19136	2209	0.221
7	20.232	39279	6191	0.454
Total		8645951	1148170	100.000