

Sample Name :Endothelin 1, human, porcine
 Cat No. :RP12758
 Lot No. :E5632220K
 Time Processed :7:21:06 AM
 Month-Day-Year Processed :11/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 27.00 | Pumps | Pump A B.Conc | 95 |
| 27.01 | Pumps | Pump A B.Conc | 5 |
| 35.00 | Pumps | Pump A B.Conc | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

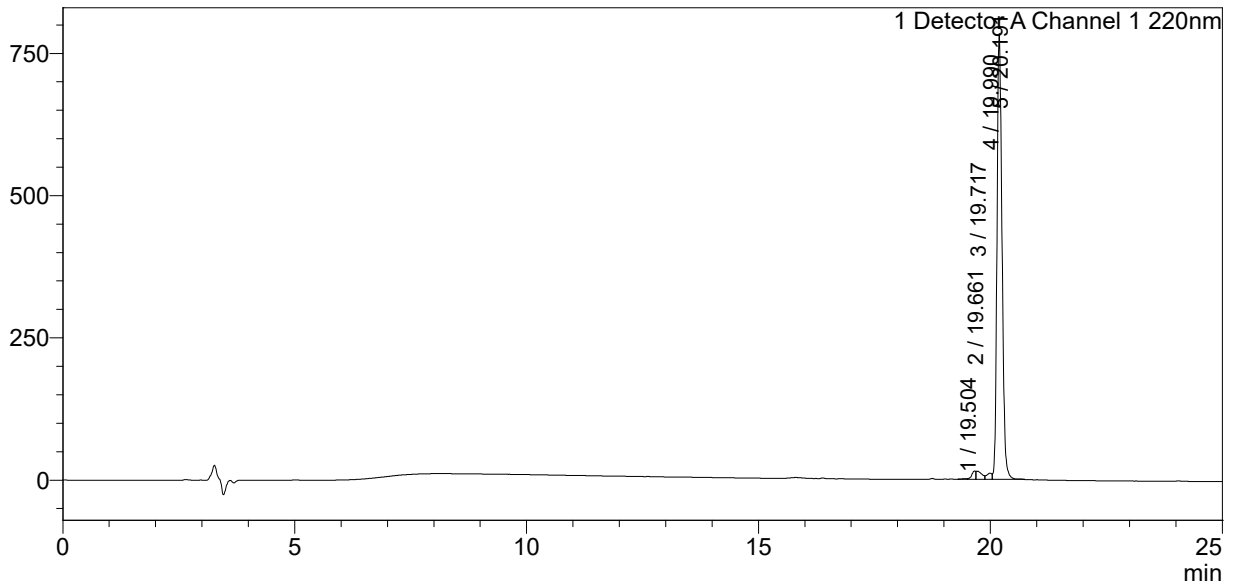

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 19.504 | 10251 | 1223 | 0.165 |
| 2 | 19.661 | 91075 | 14390 | 1.466 |
| 3 | 19.717 | 121212 | 14353 | 1.952 |
| 4 | 19.990 | 85870 | 10814 | 1.383 |
| 5 | 20.191 | 5902149 | 783539 | 95.034 |
| Total | | 6210556 | 824318 | 100.000 |