

Sample Name :N-Boc-Phe-Leu-Phe-Leu-Phe
 Cat No.: RP12950
 Lot No.:E9577119L
 Time Processed :14:38:40
 Month-Day-Year Processed :12/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
31.00	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

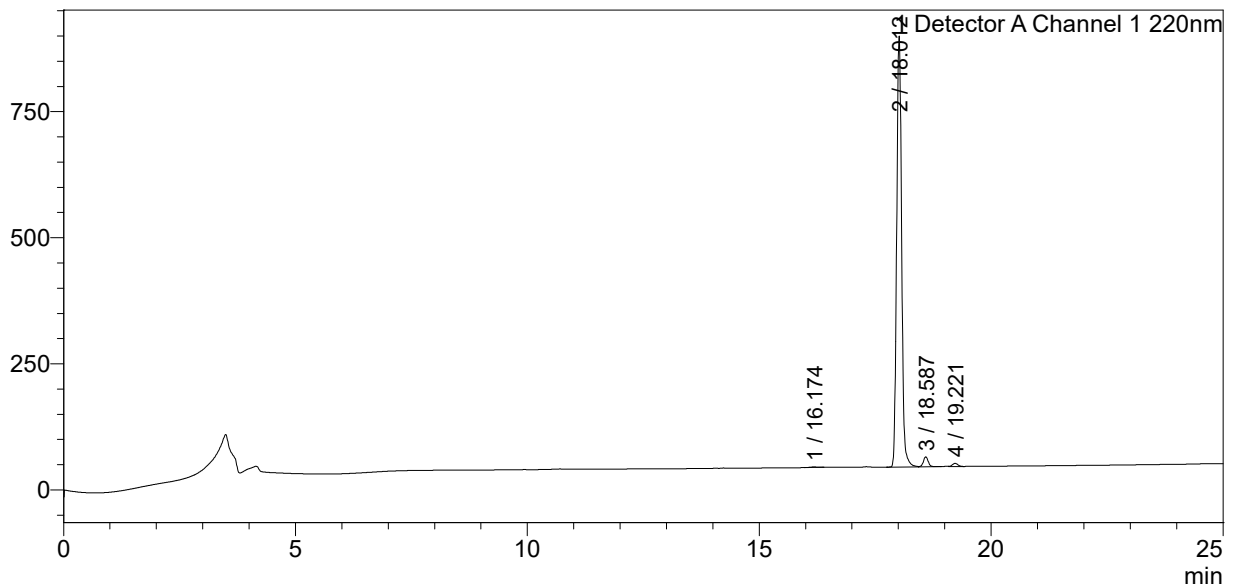

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.174	10324	993	0.157
2	18.012	6361631	855005	96.840
3	18.587	145217	19887	2.211
4	19.221	52021	6417	0.792
Total		6569193	882303	100.000