


# Mass Spectrum

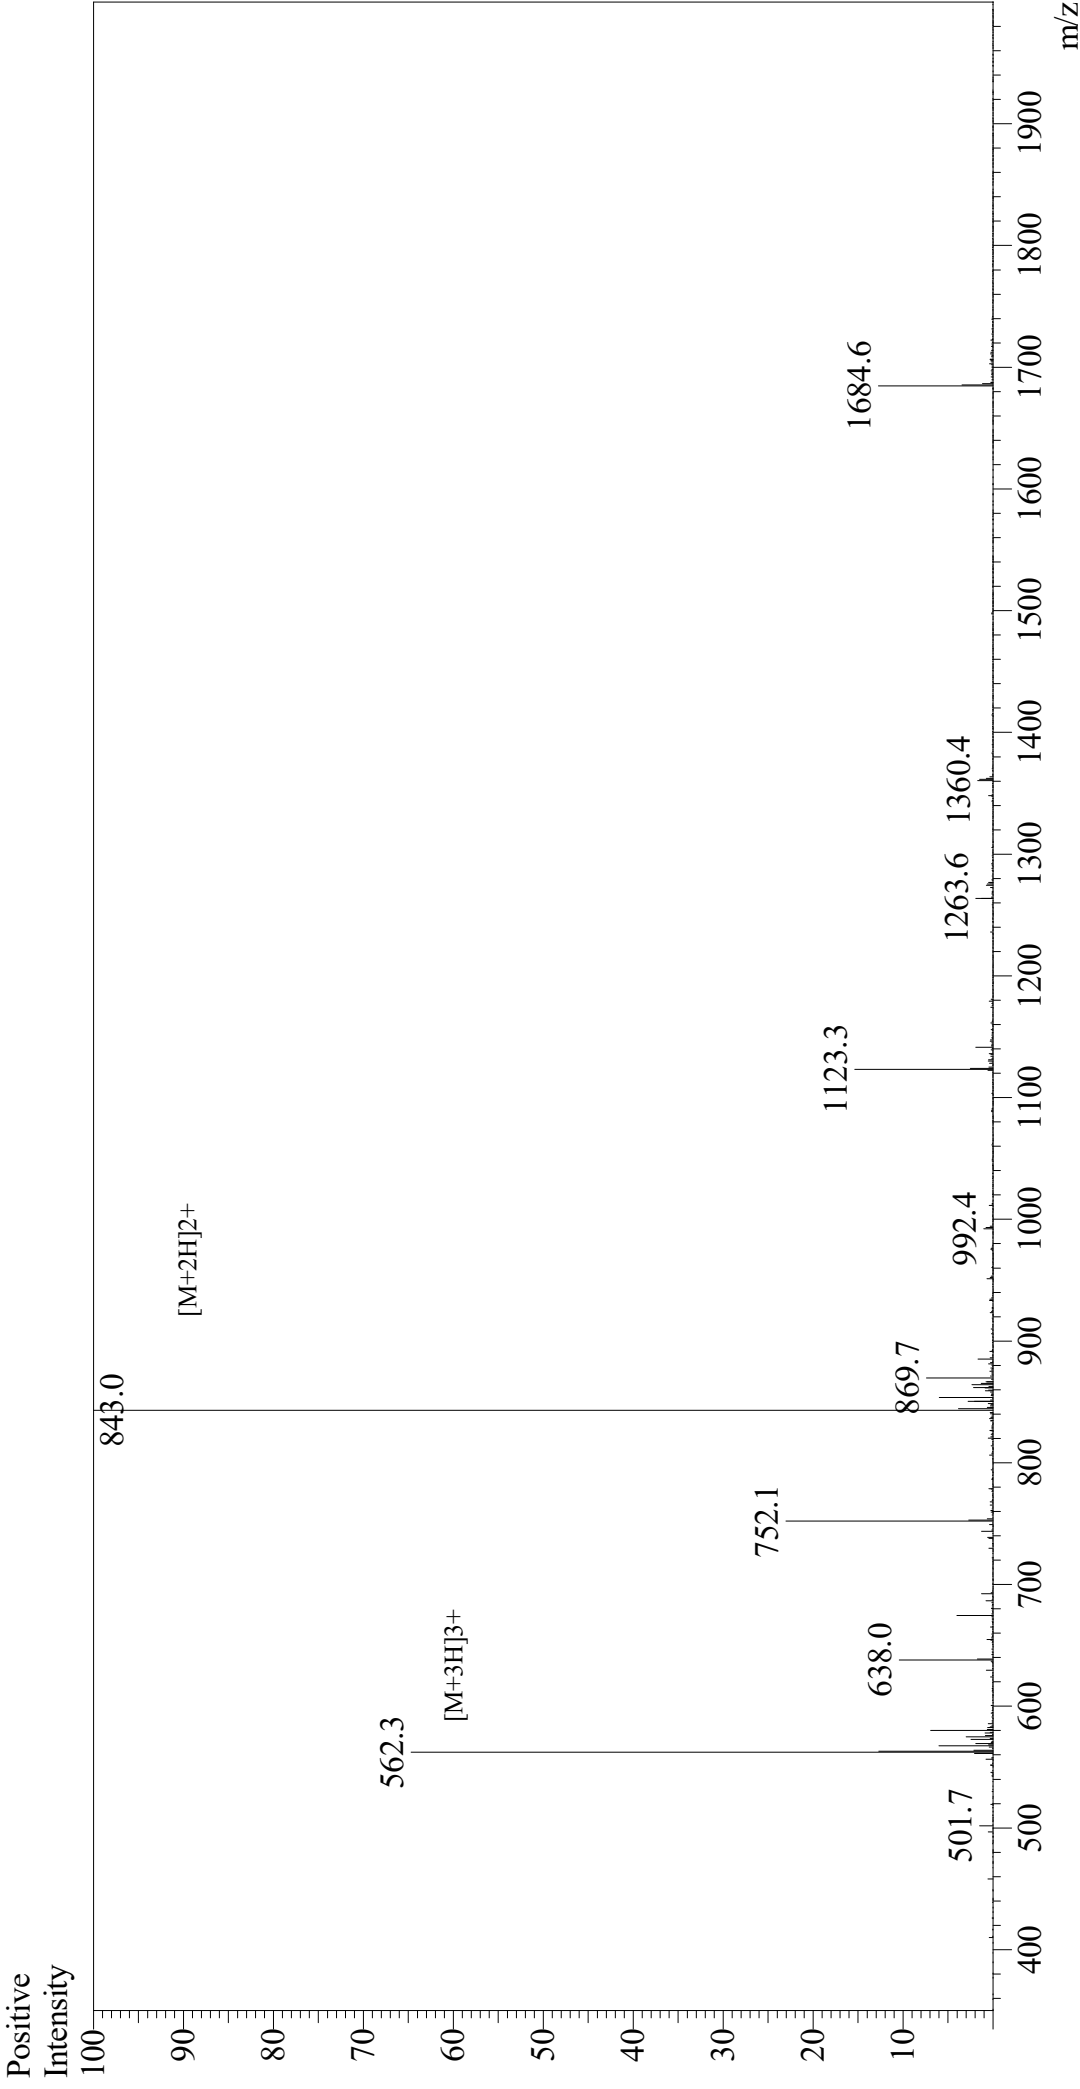

Sample Information  
Month-Day Processed : 06/23/21  
Time Processed : 7:21:34  
Injection Volume : 0.4  
Sample Name :  $\alpha$ -Factor Mating Pheromone, yeast  
Cat No : RP01002  
Lot No : E8661821F  
Theoretical MW : 1683.98  
Observed MW : 1684.0

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50% H2O/50% MeOH