

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), human
 Cat No.: RP11089
 Lot No.: E6133920B
 Time Processed : 12:12:35
 Month-Day-Year Processed : 02/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.00	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	95
35.10	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

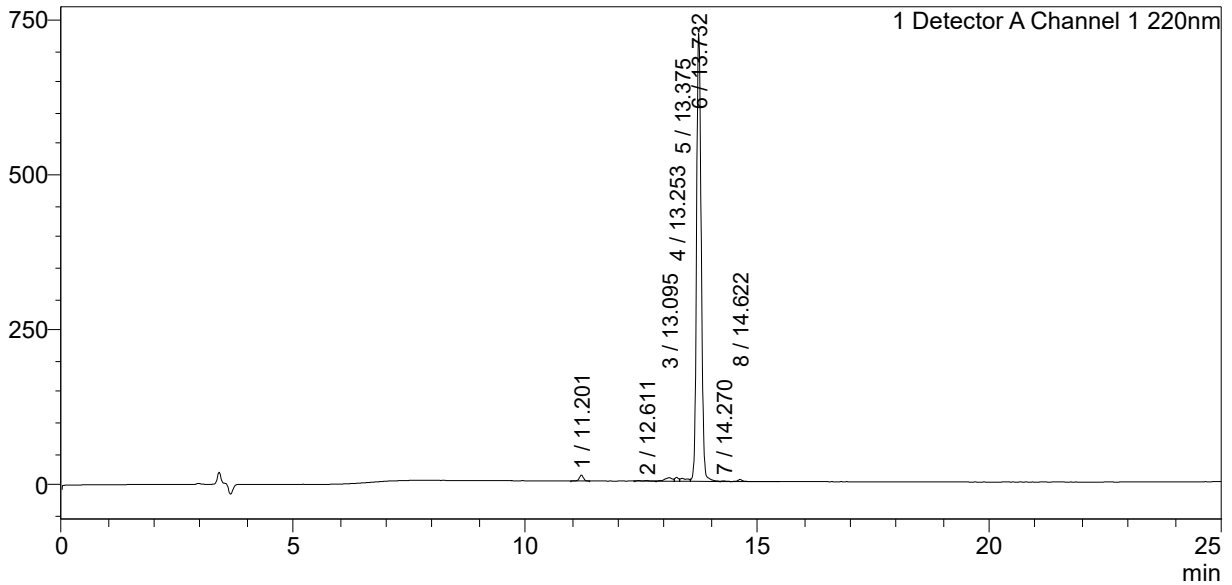

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.201	57997	9601	1.092
2	12.611	12251	889	0.231
3	13.095	62391	5767	1.175
4	13.253	39859	6190	0.750
5	13.375	50784	4617	0.956
6	13.732	5058372	722467	95.230
7	14.270	6576	792	0.124
8	14.622	23501	3280	0.442
Total		5311733	753602	100.000