

Sample Name:mTRP-2(180-188)  
 Cat No. : RP20250  
 Lot No. : E80110201  
 Time Processed : 12:34:33  
 Month-Day-Year Processed :09/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

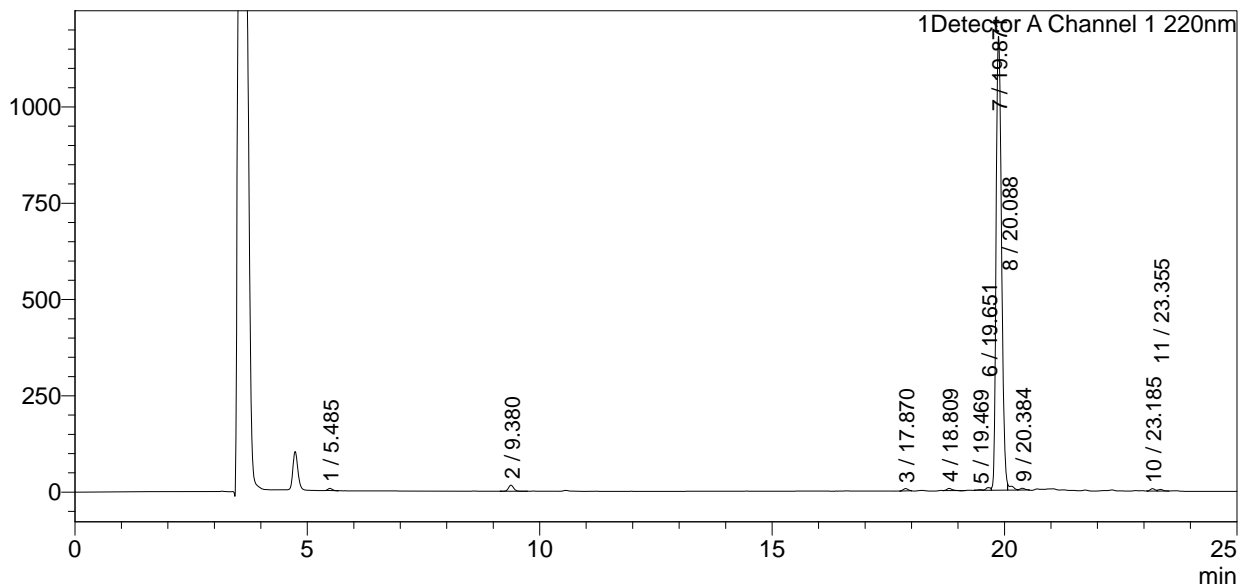

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.485	35032	5595	0.350
2	9.380	121027	15743	1.208
3	17.870	43946	6031	0.439
4	18.809	33840	5382	0.338
5	19.469	9885	1535	0.099
6	19.651	48660	6950	0.486
7	19.871	9533247	1166537	95.144
8	20.088	89392	12495	0.892
9	20.384	33100	4700	0.330
10	23.185	43637	6132	0.436
11	23.355	28054	4043	0.280
Total		10019819	1235142	100.000