

Sample Name :Somatostatin
 Cat No.: RP10226
 Lot No.: E5733519K
 Time Processed :8:35:54
 Month-Day-Year Processed :11/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

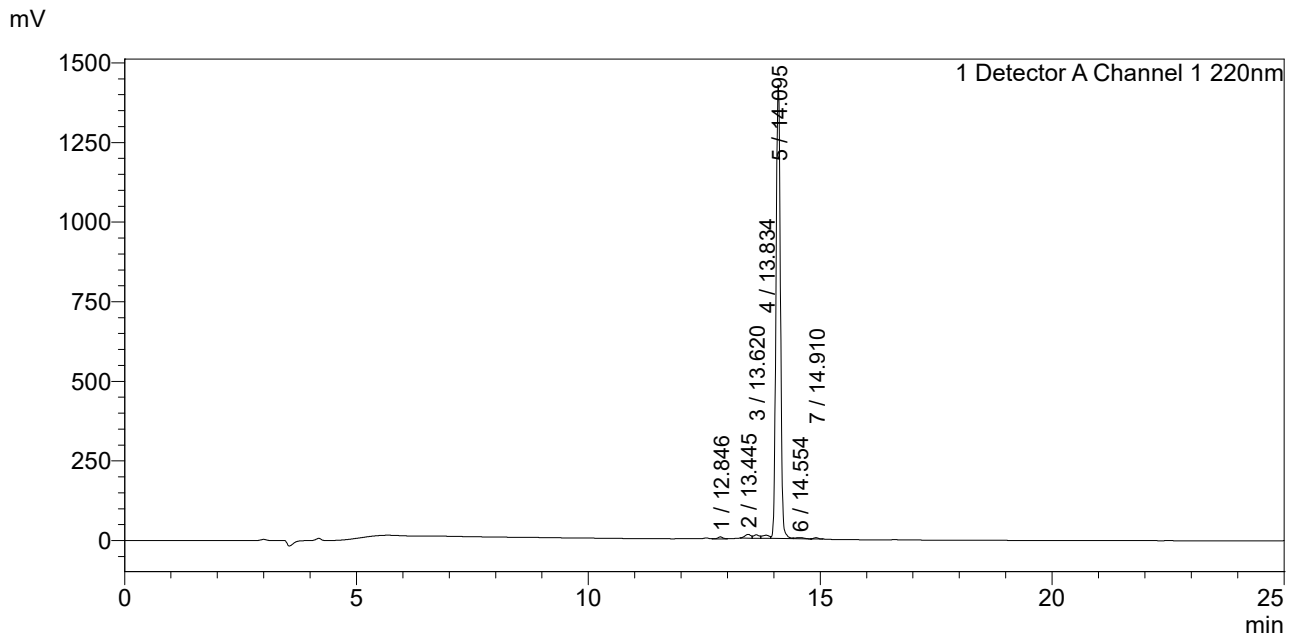

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.846	46565	6187	0.474
2	13.445	107754	12011	1.096
3	13.620	93540	10711	0.952
4	13.834	105189	9865	1.070
5	14.095	9402241	1424680	95.645
6	14.554	47874	3853	0.487
7	14.910	27172	4071	0.276
Total		9830336	1471378	100.000