

Sample Name :  $\beta$ -Amyloid (25-35)  
 Cat No.: RP10008  
 Lot No.: E38716201  
 Time Processed :8:30:00  
 Month-Day-Year Processed :09/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

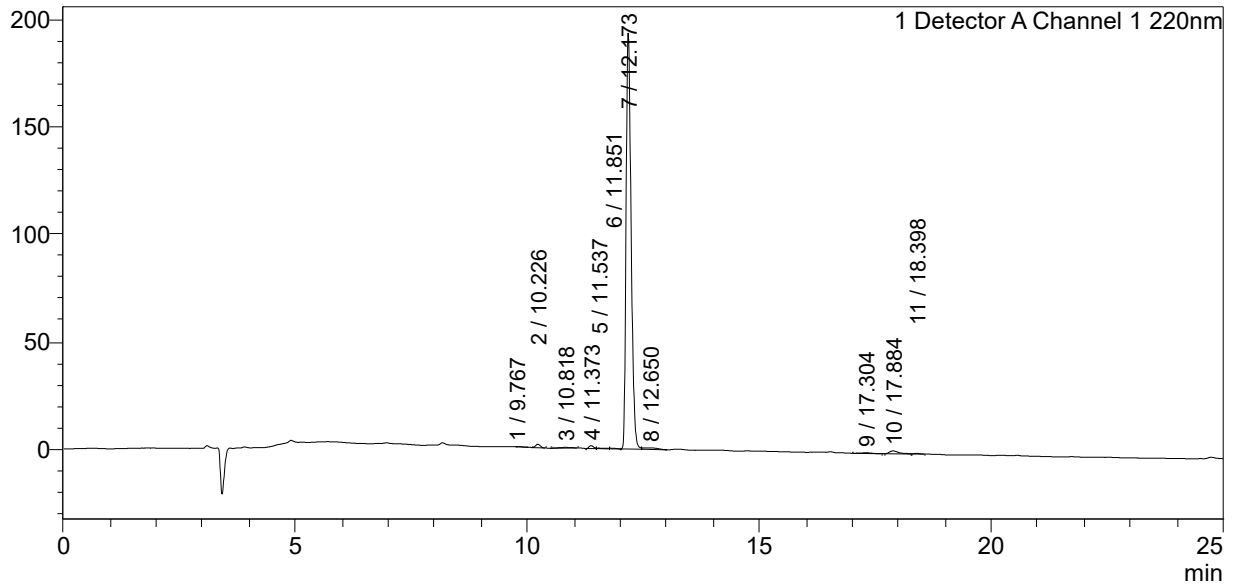

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.767	534	37	0.035
2	10.226	11155	1631	0.724
3	10.818	5635	331	0.366
4	11.373	9081	1395	0.590
5	11.537	3329	272	0.216
6	11.851	1607	220	0.104
7	12.173	1464136	193754	95.046
8	12.650	15389	778	0.999
9	17.304	5821	338	0.378
10	17.884	20459	1387	1.328
11	18.398	3306	300	0.215
Total		1540452	200443	100.000