


Mass Spectrum

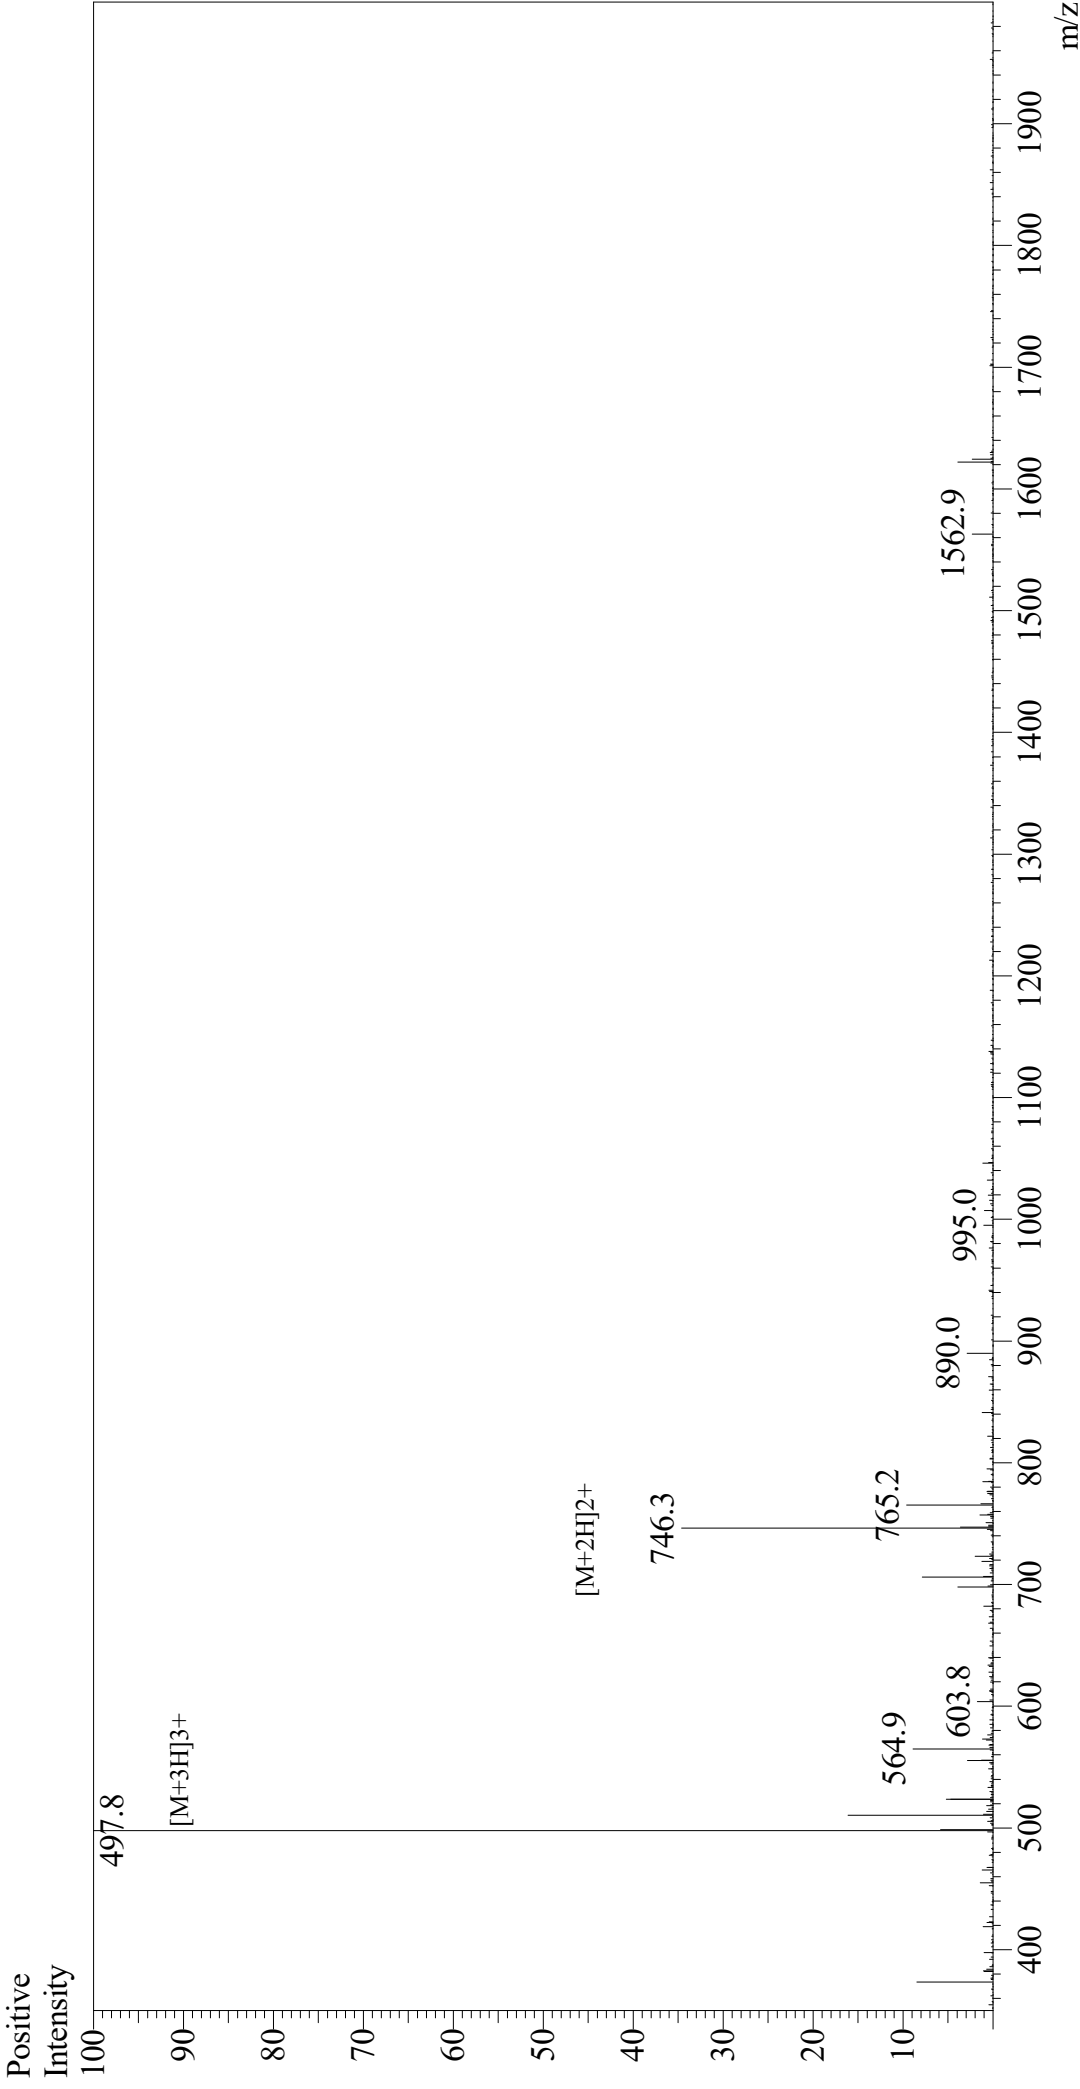

Sample Information
Month-Day Processed : 06/10/21
Time Processed : 4:38:41 PM
Injection Volume : 0.4
Sample Name : SV40 T-Ag-derived NLS peptide
Cat No: RP20513
Lot No: E9915721F
Theoretical MW : 1490.80
Observed MW : 1490.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH