

Sample Name :Cys-TAT(47-57)
 Cat. No. :RP20343
 Lot. No. :E4942319I
 Time Processed :17:35:51
 Month-Day-Year Processed :09/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
25.00	Pumps	Pump B Conc.	60	
25.01	Pumps	Pump B Conc.	80	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

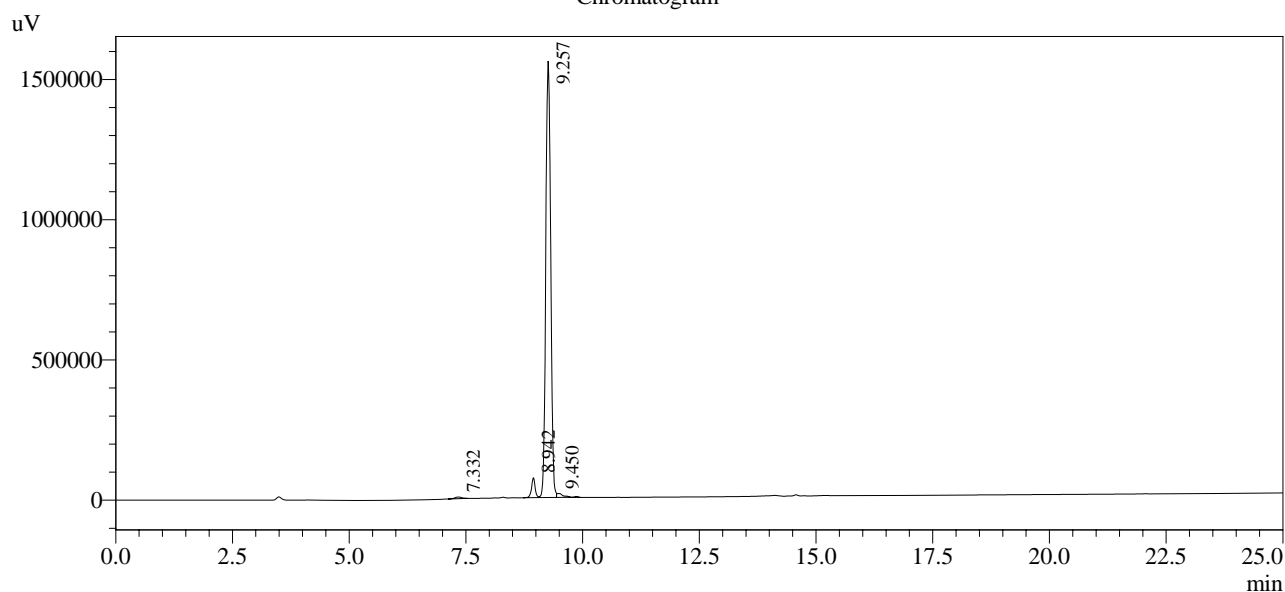

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.332	60121	5770	0.500
2	8.942	380215	70548	3.165
3	9.257	11424182	1555791	95.101
4	9.450	148187	14111	1.234
Total		12012705	1646219	100.000