

Sample Name :Mtrp-2(180-188)
 Cat. No. : RP20250
 Lot. No. : PE2941810
 Time Processed : 9:01:31
 Month-Day-Year Processed : 10/19/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

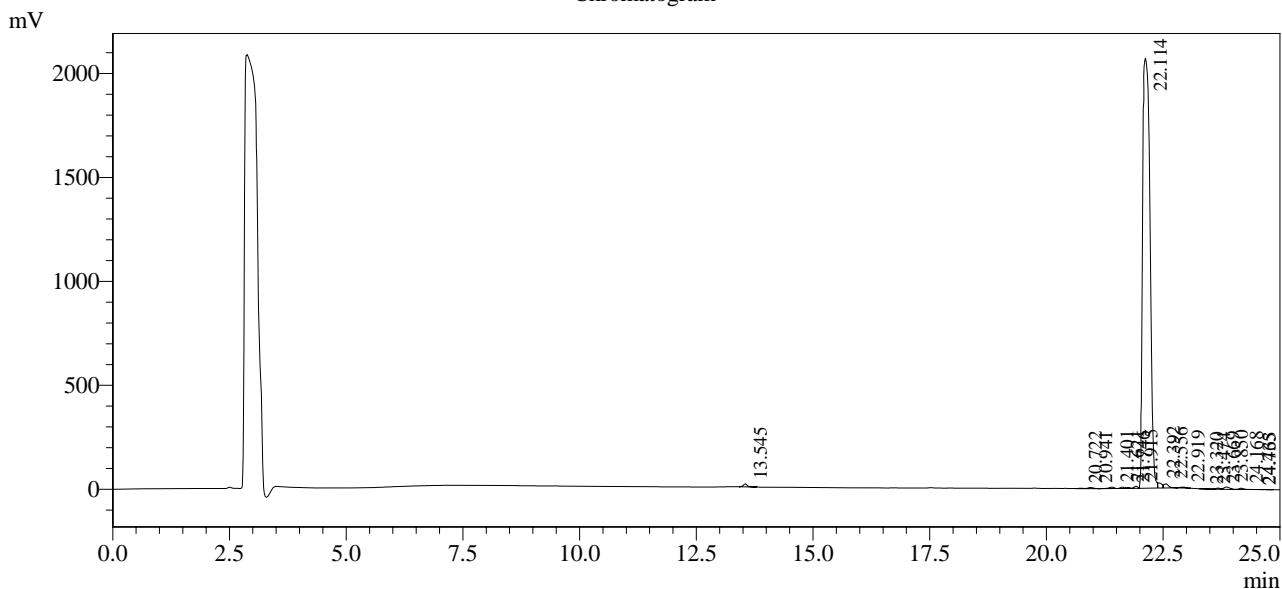

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.545	84831	14136	0.360
2	20.722	12895	1865	0.055
3	20.941	40719	5346	0.173
4	21.401	51565	6696	0.219
5	21.621	37957	6430	0.161
6	21.746	22692	4438	0.096
7	21.915	52546	10131	0.223
8	22.114	22752150	2068477	96.593
9	22.392	149355	25035	0.634
10	22.556	138364	19860	0.587
11	22.919	39086	5130	0.166
12	23.320	2766	570	0.012
13	23.474	1082	232	0.005
14	23.669	32013	5532	0.136
15	23.850	95217	11115	0.404
16	24.168	37931	5671	0.161
17	24.463	2601	345	0.011
18	24.735	1005	155	0.004
Total		23554774	2191164	100.000