

Sample Name :Neurotensin
 Cat No.: RP10439
 Lot No.: E2784420E
 Time Processed :18:37:50
 Month-Day-Year Processed :05/31/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

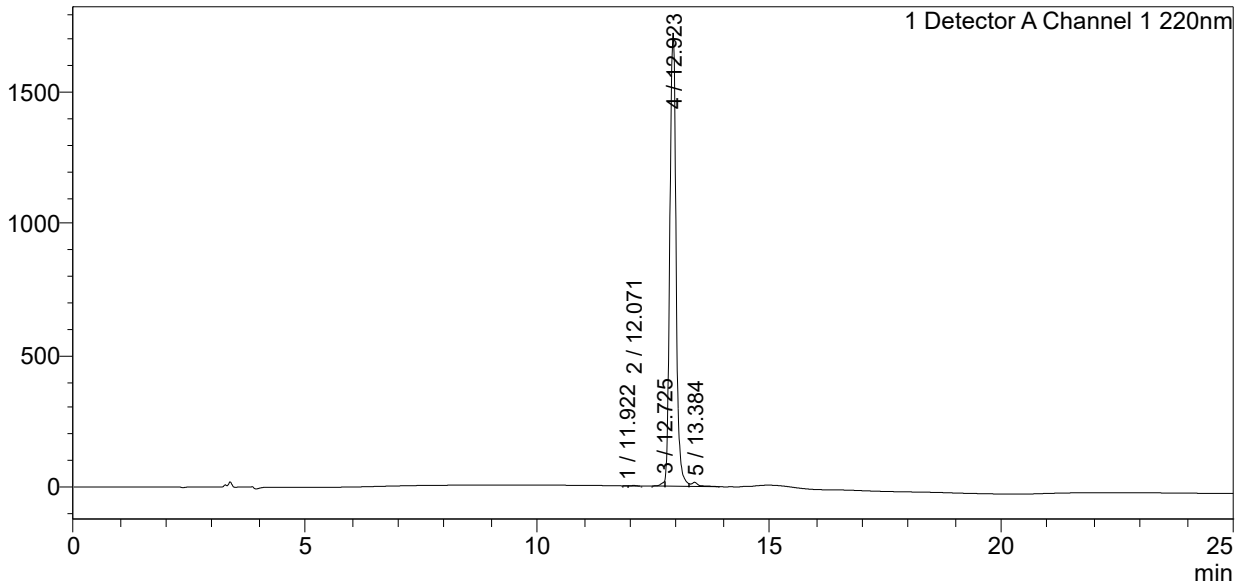

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.922	2058	388	0.013
2	12.071	11343	1618	0.069
3	12.725	73988	14497	0.453
4	12.923	16055511	1723466	98.317
5	13.384	187465	15564	1.148
Total		16330365	1755534	100.000