

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), human, porcine

Cat No. :RP11927

Lot No. :E38686201

Time Processed :9:22:10

Month-Day-Year Processed :08/25/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010324

<Chromatogram>

mV

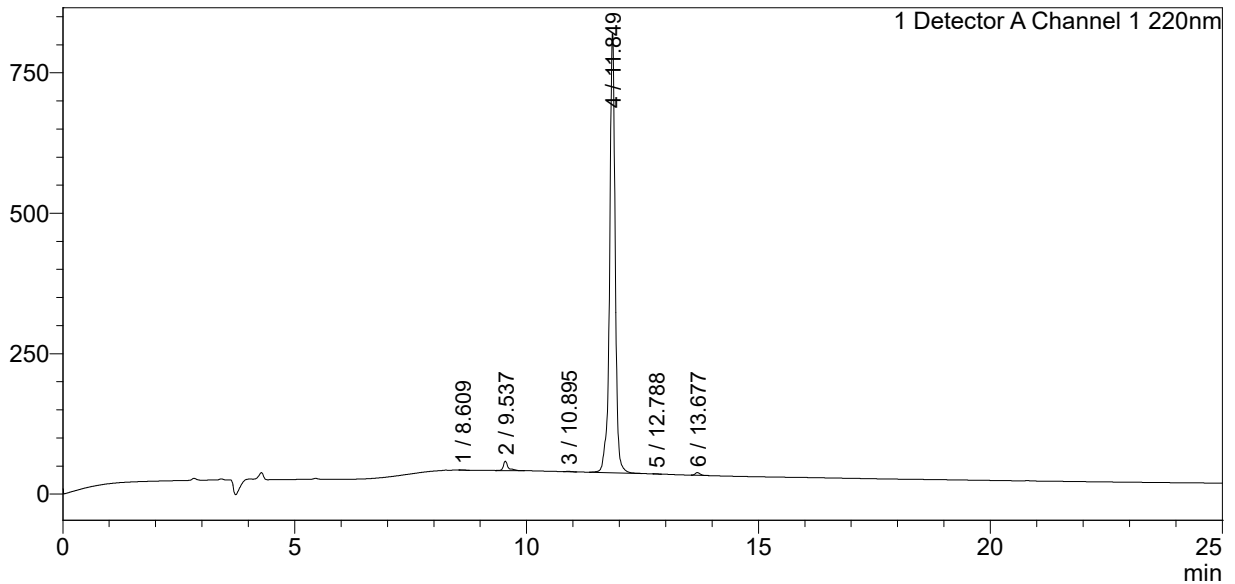

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.609	2337	464	0.035
2	9.537	121929	16907	1.821
3	10.895	4852	662	0.072
4	11.849	6528492	781846	97.515
5	12.788	2010	411	0.030
6	13.677	35249	4913	0.527
Total		6694869	805204	100.000