

Sample Name :BDC2.5 mimotope 1040-31
 Cat. No. : RP20518
 Lot. No. : PE3451902
 Time Processed : 14:20:19
 Month-Day-Year Processed : 02/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

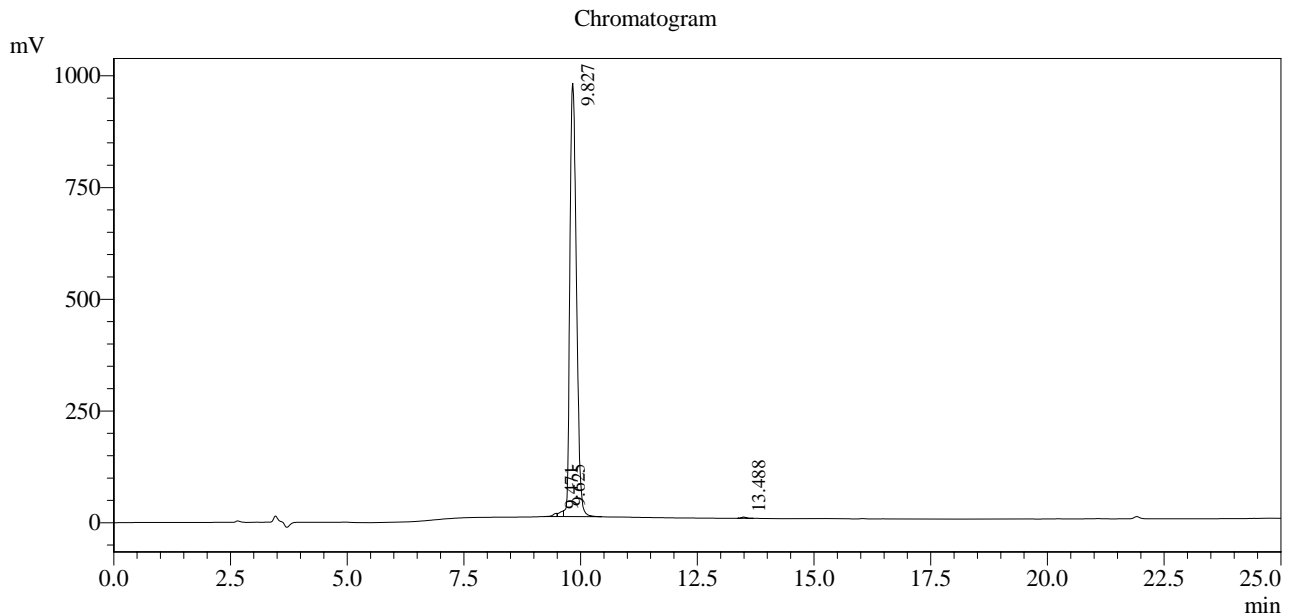

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.471	45036	7088	0.467
2	9.625	79557	12666	0.826
3	9.827	9491287	969717	98.519
4	13.488	18060	2656	0.187
Total		9633940	992127	100.000