

Sample Name :Osteogenic Growth Peptide, OGP  
 Cat No.: RP20311  
 Lot No.: E4919119I  
 Time Processed:10:39:27  
 Month-Day-Year Processed:09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

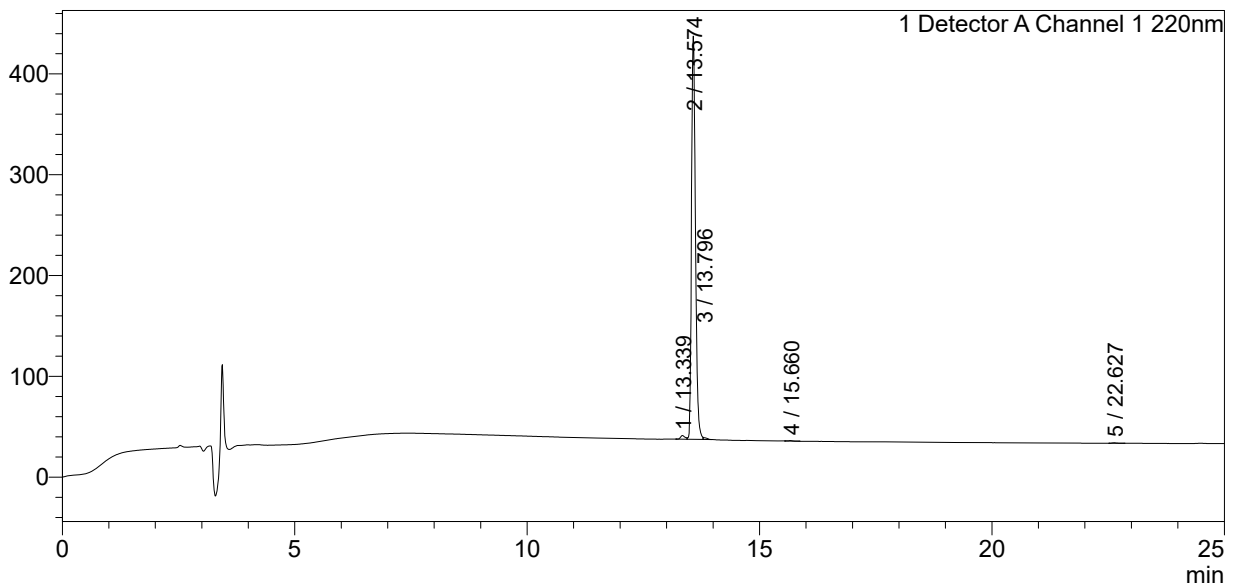

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.339	24775	3672	1.035
2	13.574	2353881	399977	98.292
3	13.796	9585	1851	0.400
4	15.660	3223	540	0.135
5	22.627	3313	461	0.138
Total		2394777	406500	100.000