

Sample Name : -Amyloid (25-35)
 Cat No: RP10008
 Lot No : E7244721A
 Time Processed :12:21:27 PM
 Month-Day-Year Processed :01/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

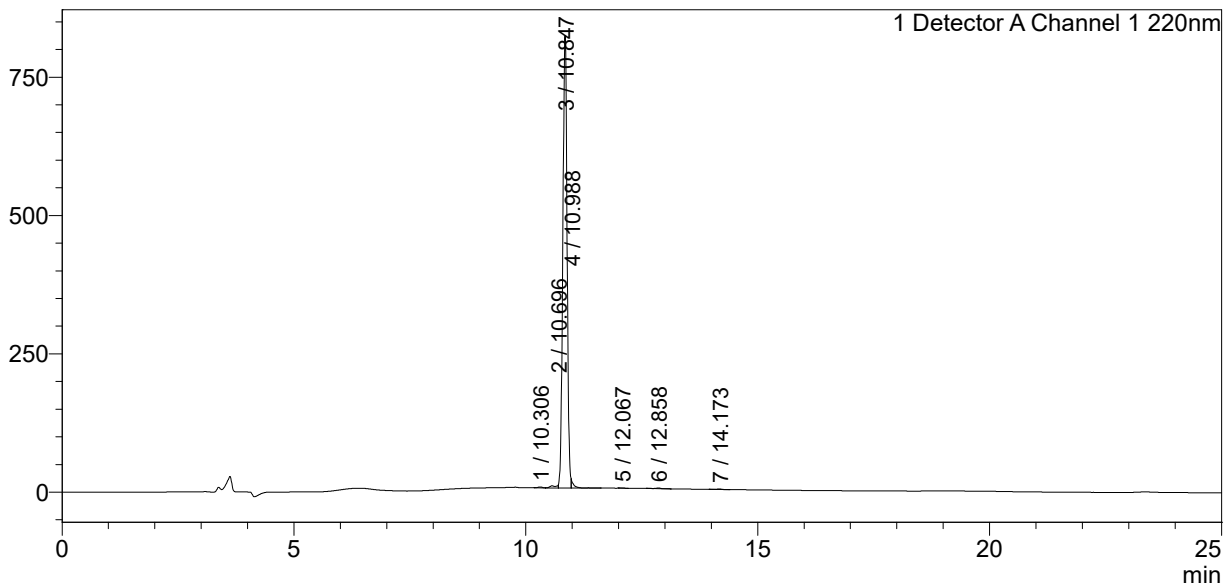

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.306	10690	1692	0.199
2	10.696	40935	4177	0.762
3	10.847	5252264	817613	97.735
4	10.988	52824	13936	0.983
5	12.067	2462	501	0.046
6	12.858	8200	1307	0.153
7	14.173	6597	958	0.123
Total		5373971	840184	100.000