


Mass Spectrum

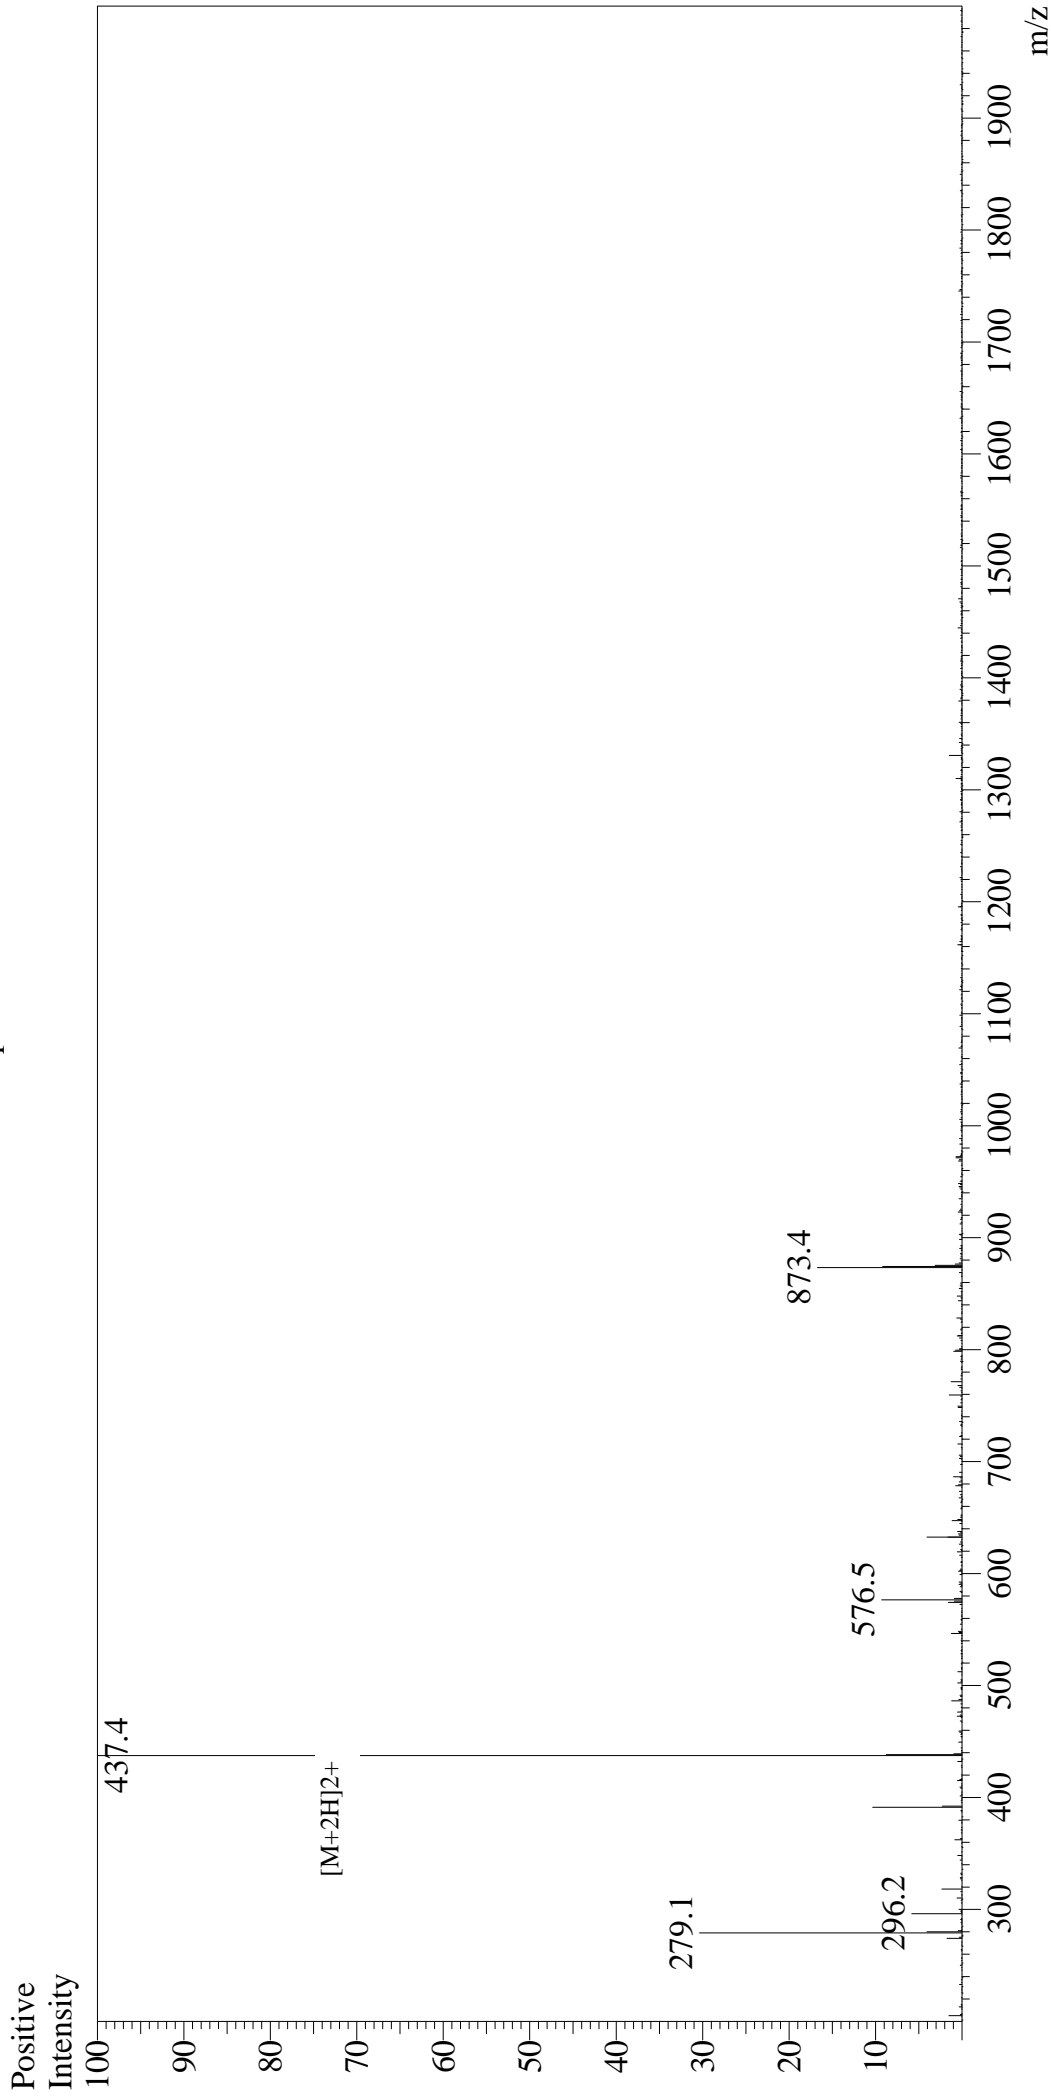

Sample Information

User : Gary
Month-Day Processed : 09/18/19
Time Processed : 9:30:40
Injection Volume : 0.3
Sample Name : A-779
Cat No. : RP11249
Lot No. : E4725119I
Theoretical MW : 873.00
Observed MW : 872.8

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH