

Sample Name : C-Myc Peptide  
 Cat No : RP11731  
 Lot No : E3021221D  
 Time Processed : 11:29:35 PM  
 Month-Day-Year Processed : 04/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010011

<Chromatogram>

mV

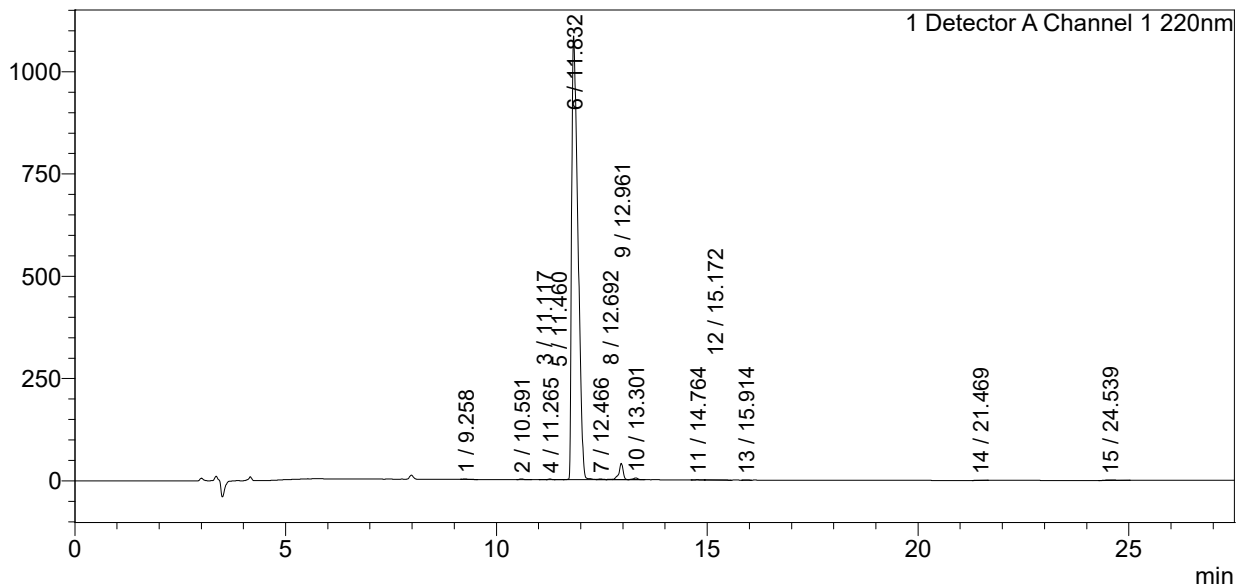

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.258	9751	1370	0.084
2	10.591	11188	1916	0.096
3	11.117	3410	615	0.029
4	11.265	9717	1596	0.084
5	11.460	5365	646	0.046
6	11.832	11233807	1083783	96.549
7	12.466	8014	1130	0.069
8	12.692	4771	833	0.041
9	12.961	271117	39544	2.330
10	13.301	34661	4383	0.298
11	14.764	6728	810	0.058
12	15.172	6492	423	0.056
13	15.914	1282	206	0.011
14	21.469	4312	434	0.037
15	24.539	24757	1422	0.213
Total		11635372	1139110	100.000