

Sample Name :LAH4  
 Cat. No. : RP20096  
 Lot. No. : E0102819L  
 Time Processed :5:23:09  
 Month-Day-Year Processed : 12/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

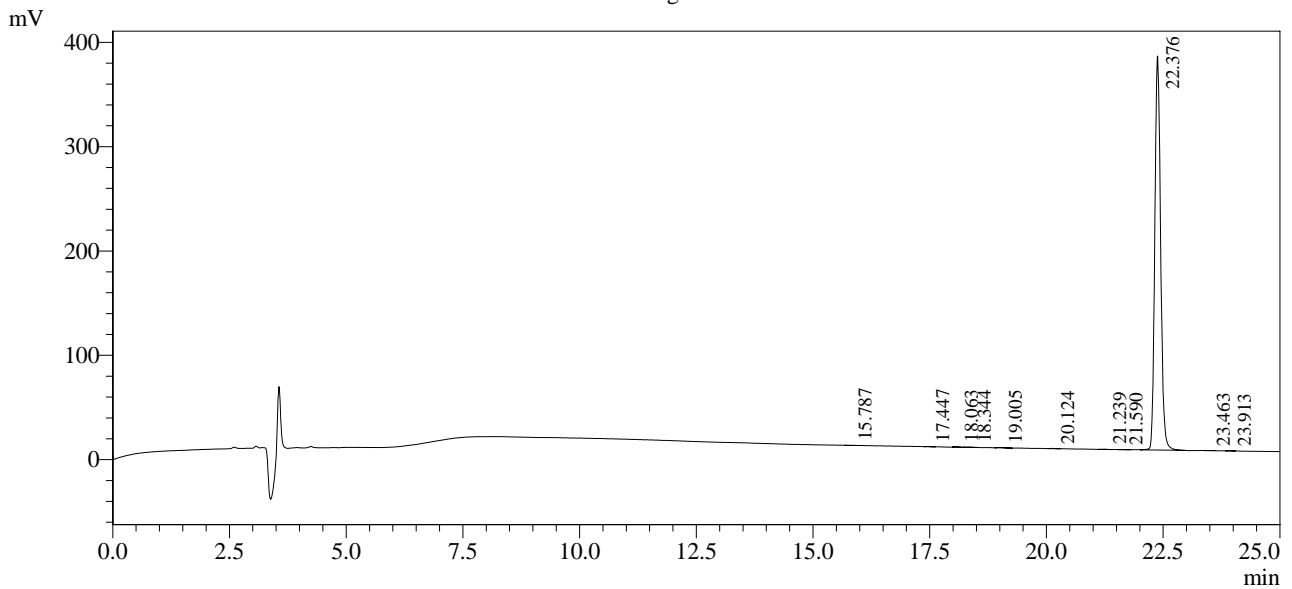

1 Det.A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.787	3093	311	0.094
2	17.447	1042	188	0.032
3	18.063	3091	495	0.094
4	18.344	2652	301	0.080
5	19.005	3618	430	0.109
6	20.124	1581	254	0.048
7	21.239	1449	225	0.044
8	21.590	1185	170	0.036
9	22.376	3283223	377746	99.364
10	23.463	1546	199	0.047
11	23.913	1768	302	0.054
Total		3304249	380620	100.000