

Sample Name :[Arg8]-Vasopressin (AVP)
 Cat No. :RP20275
 Lot No. :E2613420G
 Time Processed :8:48:03 AM
 Month-Day-Year Processed :07/31/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

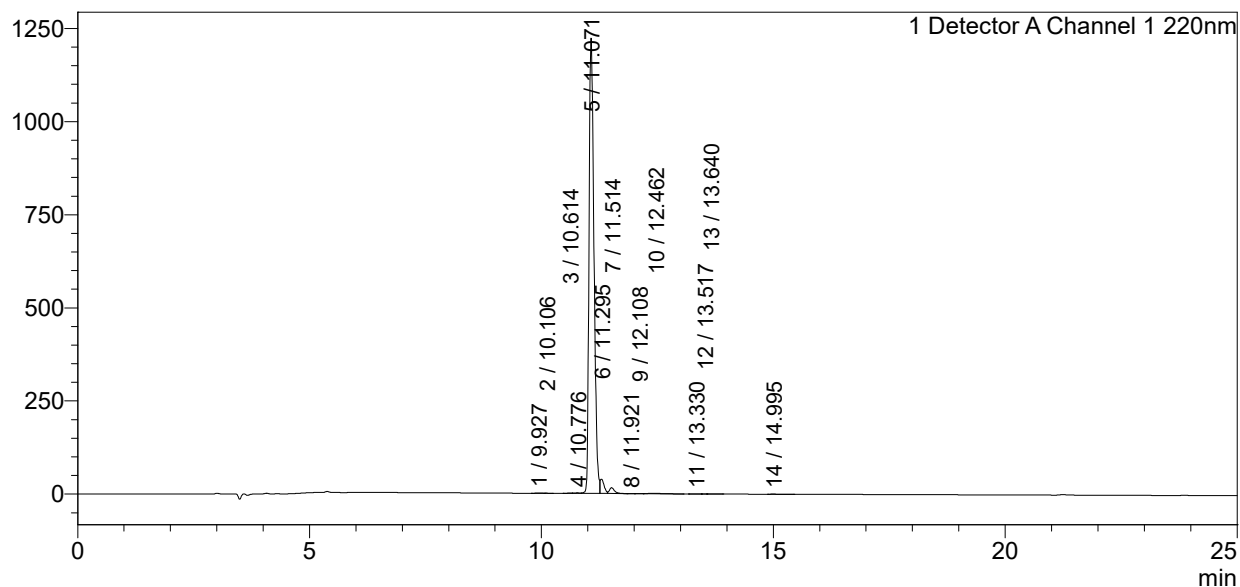

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.927	8384	1027	0.088
2	10.106	2546	341	0.027
3	10.614	5523	861	0.058
4	10.776	13398	1423	0.141
5	11.071	9081364	1222748	95.621
6	11.295	226057	38510	2.380
7	11.514	118185	15651	1.244
8	11.921	1004	126	0.011
9	12.108	3495	350	0.037
10	12.462	25935	869	0.273
11	13.330	2623	304	0.028
12	13.517	1033	157	0.011
13	13.640	2740	290	0.029
14	14.995	4988	469	0.053
Total		9497276	1283128	100.000