

Sample Name : C-telopeptide
 Cat. No. : RP10566
 Lot. No. : E6997319J
 Time Processed : 10:53:28
 Month-Day-Year Processed : 10/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	20	
40.00	Pumps	Pump A B.Conc	20	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

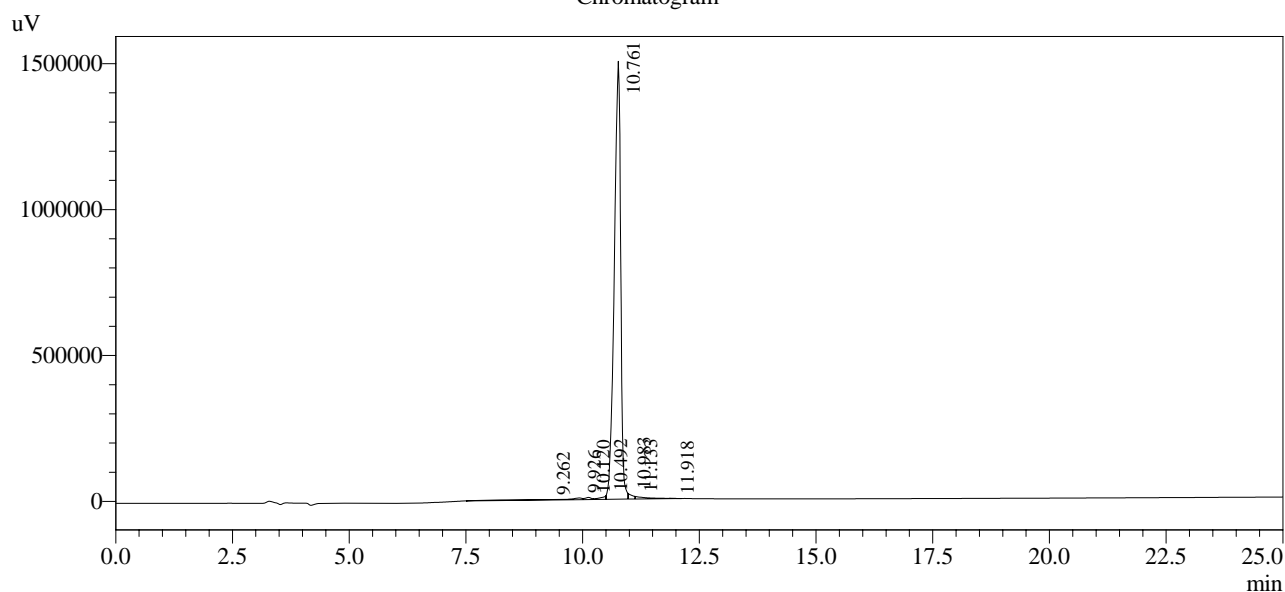

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.262	179131	1877	1.195
2	9.926	100451	5833	0.670
3	10.120	64874	7274	0.433
4	10.492	90789	10939	0.606
5	10.761	14283021	1500784	95.302
6	10.983	114213	18473	0.762
7	11.133	153788	8513	1.026
8	11.918	792	215	0.005
Total		14987058	1553908	100.000