

Sample Name : CREBtide
 Cat. No. : RP10142
 Lot. No. : E4880220F
 Time Processed : 3:32:04
 Month-Day-Year Processed : 07/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

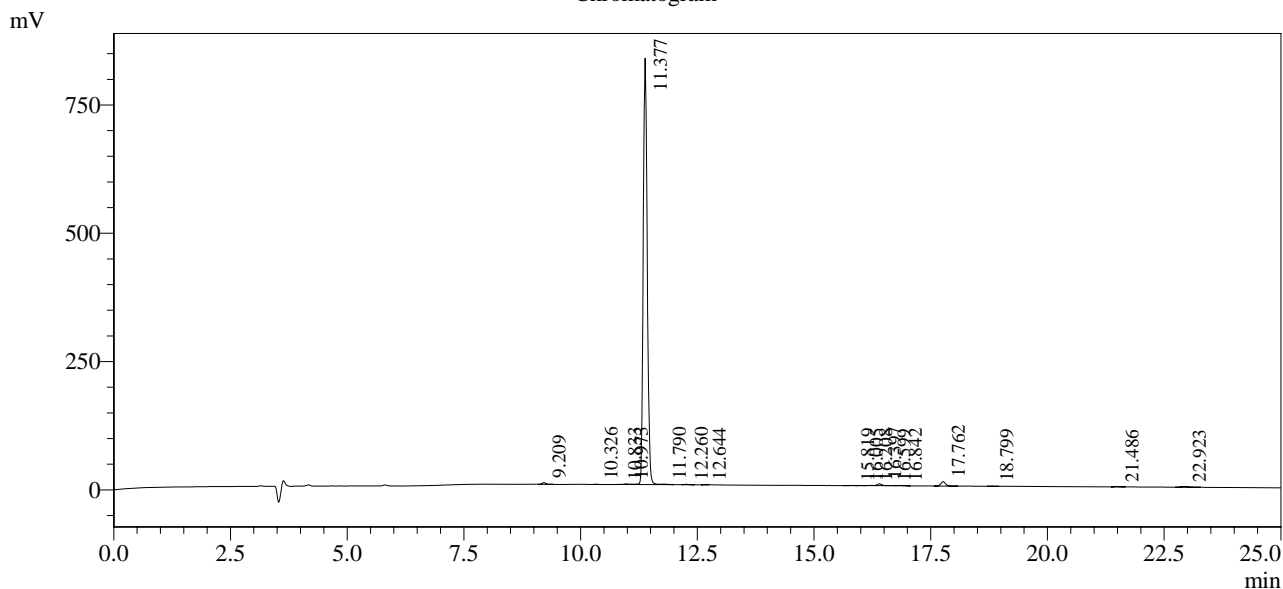

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.209	18513	3365	0.360
2	10.326	3624	594	0.070
3	10.833	2207	273	0.043
4	10.973	9855	1331	0.191
5	11.377	4990463	830789	96.943
6	11.790	2191	466	0.043
7	12.260	5065	832	0.098
8	12.644	1086	243	0.021
9	15.819	1961	276	0.038
10	16.005	1402	200	0.027
11	16.208	3127	345	0.061
12	16.397	23340	3470	0.453
13	16.599	1092	150	0.021
14	16.842	4768	396	0.093
15	17.762	59620	8483	1.158
16	18.799	2292	352	0.045
17	21.486	3560	500	0.069
18	22.923	13669	1270	0.266
Total		5147836	853333	100.000