

Sample Name :Systemin
 Cat No. :RP10622
 Lot No. :E4744119I
 Time Processed :10:57:11 AM
 Month-Day-Year Processed :09/27/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
30.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

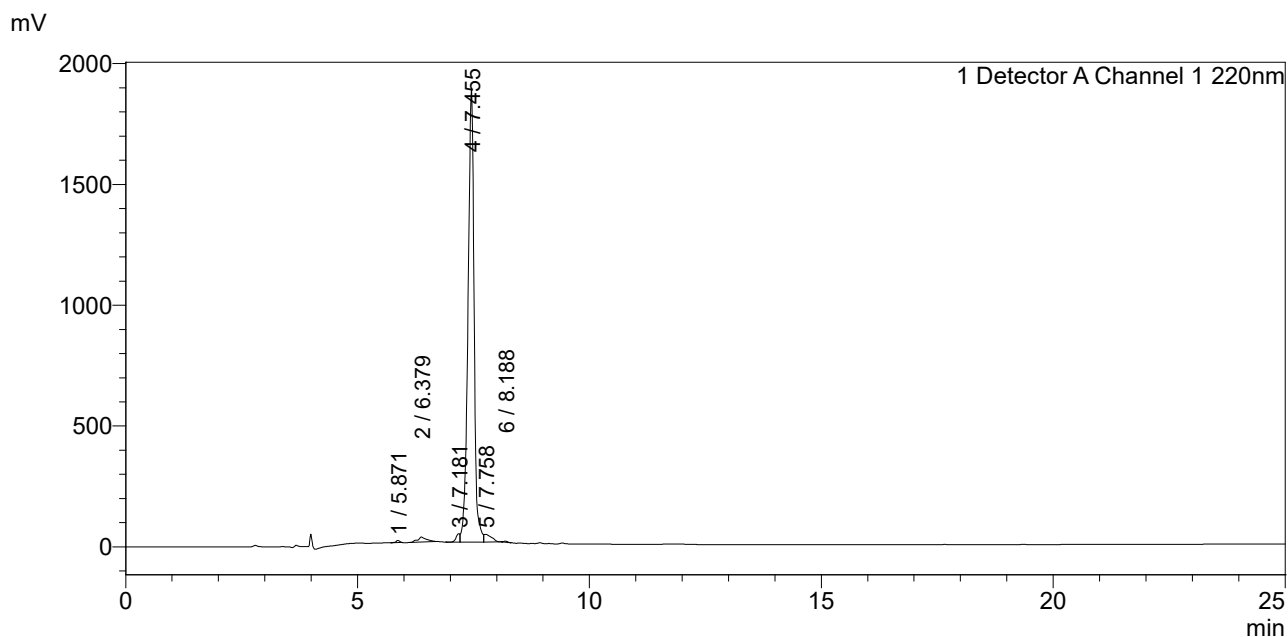

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.871	47612	9031	0.263
2	6.379	281103	20896	1.555
3	7.181	200574	34641	1.110
4	7.455	17172911	1878564	95.025
5	7.758	346262	31821	1.916
6	8.188	23541	5135	0.130
Total		18072002	1980088	100.000