

Sample Name :Somatostatin
 Cat No. :RP10226
 Lot No. :E4117321H
 Time Processed :12:33:18
 Month-Day-Year Processed :08/11/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

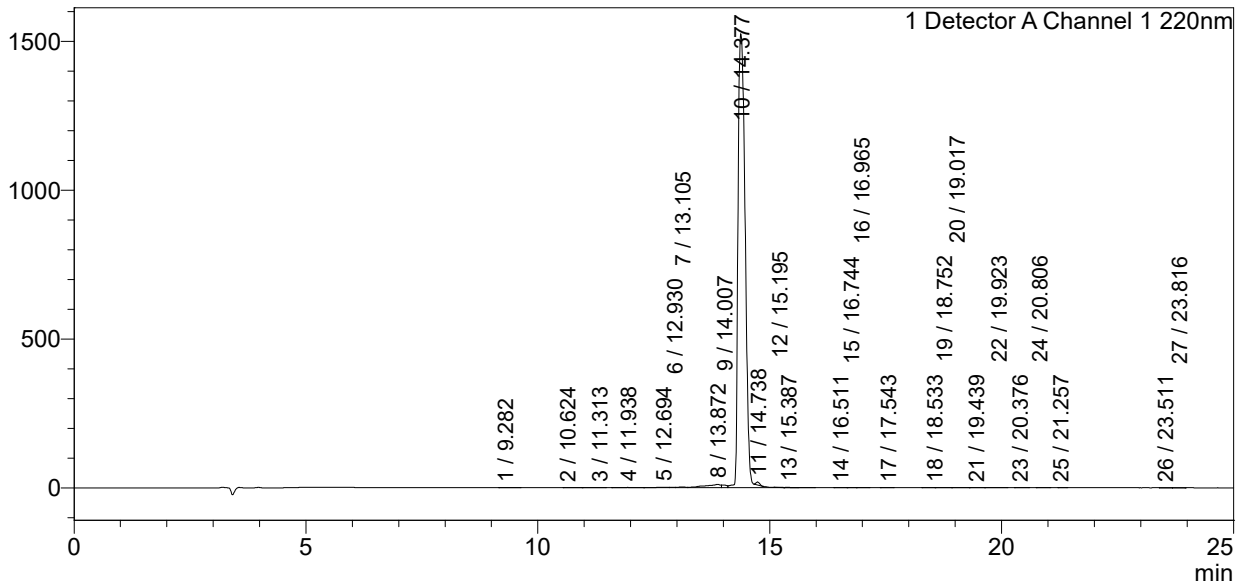

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.282	1587	118	0.009
2	10.624	1354	101	0.008
3	11.313	2164	142	0.013
4	11.938	12488	557	0.075
5	12.694	17888	948	0.107
6	12.930	6172	787	0.037
7	13.105	26778	2647	0.160
8	13.872	252145	10998	1.506
9	14.007	66485	8770	0.397
10	14.377	16235667	1525084	96.993
11	14.738	54012	10429	0.323
12	15.195	6148	988	0.037
13	15.387	2541	335	0.015
14	16.511	2814	204	0.017

Peak#	Ret. Time	Area	Height	Area%
15	16.744	2212	222	0.013
16	16.965	2075	186	0.012
17	17.543	1498	180	0.009
18	18.533	4682	481	0.028
19	18.752	11458	601	0.068
20	19.017	8794	458	0.053
21	19.439	5124	389	0.031
22	19.923	5706	290	0.034
23	20.376	2492	263	0.015
24	20.806	1191	98	0.007
25	21.257	1143	342	0.007
26	23.511	3232	371	0.019
27	23.816	1116	106	0.007
Total		16738967	1566096	100.000