

Sample Name :Moth Cytochrome C (MCC) (88-103)

Cat. No. : RP12808

Lot. No. : E9573819L

Time Processed :13:35:29

Month-Day-Year Processed : 12/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

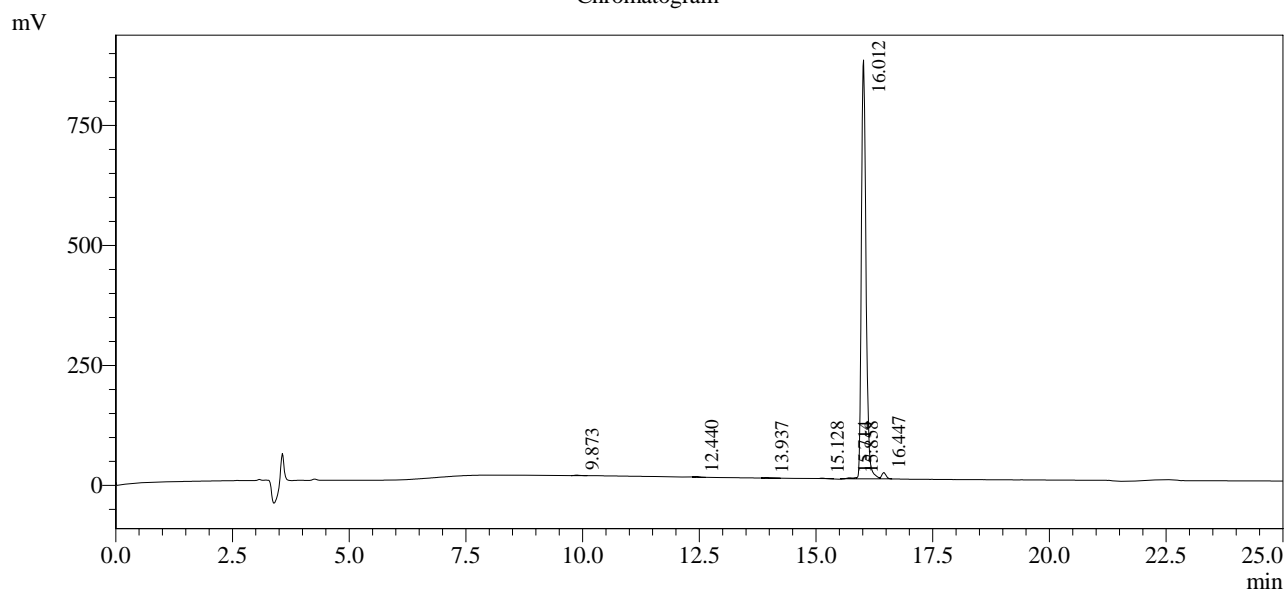

1 Det.A Ch1 / 220nm
Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.873	7204	917	0.117
2	12.440	5911	877	0.096
3	13.937	3711	521	0.060
4	15.128	6174	1002	0.100
5	15.714	15178	1988	0.247
6	15.858	9154	2455	0.149
7	16.012	6026183	872754	97.901
8	16.447	81884	13196	1.330
Total		6155398	893709	100.000