

Sample Name : Neuropeptide Y(1-36)
 Cat.No : RP20520
 Lot.No : E8981020J
 Time Processed: 0:27:32
 Year-Month-Day: 2020/11/1

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010015

<Chromatogram>

mV

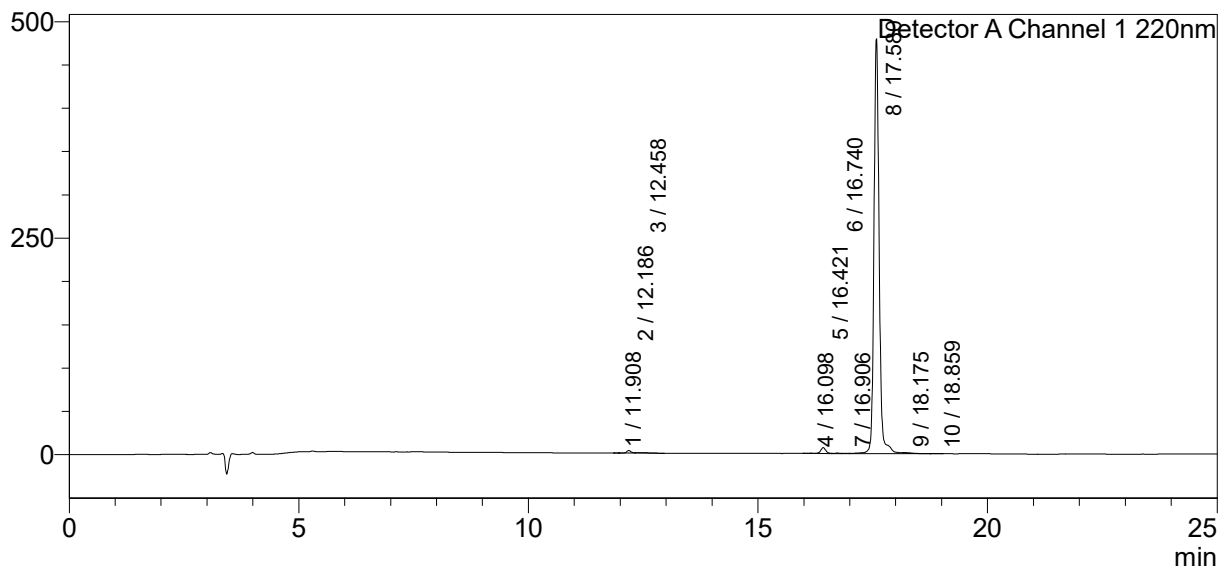

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.908	159	28	0.004
2	12.186	19660	2899	0.507
3	12.458	12854	608	0.332
4	16.098	571	104	0.015
5	16.421	53372	6700	1.377
6	16.740	4618	438	0.119
7	16.906	4152	440	0.107
8	17.580	3775836	478996	97.443
9	18.175	1622	88	0.042
10	18.859	2055	237	0.053
Total		3874898	490539	100.000