

Sample Name : Dermaseptin
 Cat. No. :RP11228
 Lot. No. :PE5351811
 Time Processed : 7:32:57
 Month-Day-Year Processed : 12/03/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

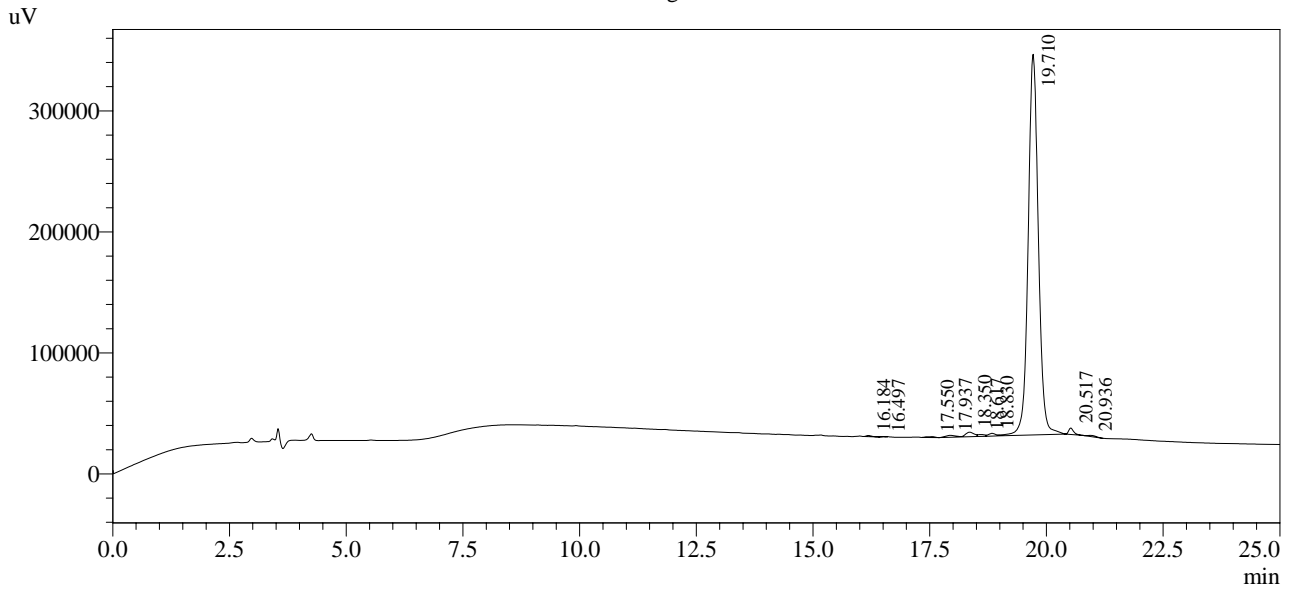

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.184	7343	948	0.148
2	16.497	1779	343	0.036
3	17.550	8916	702	0.180
4	17.937	23595	1561	0.476
5	18.350	47044	3738	0.949
6	18.617	15788	1512	0.319
7	18.830	24638	2304	0.497
8	19.710	4775373	314654	96.355
9	20.517	39410	5303	0.795
10	20.936	12140	921	0.245
Total		4956026	331987	100.000