

Sample Name :Orexin B, rat, mouse  
 Cat No.: RP10416  
 Lot No.: E4810119I  
 Time Processed:12:15:57  
 Month-Day-Year Processed:09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

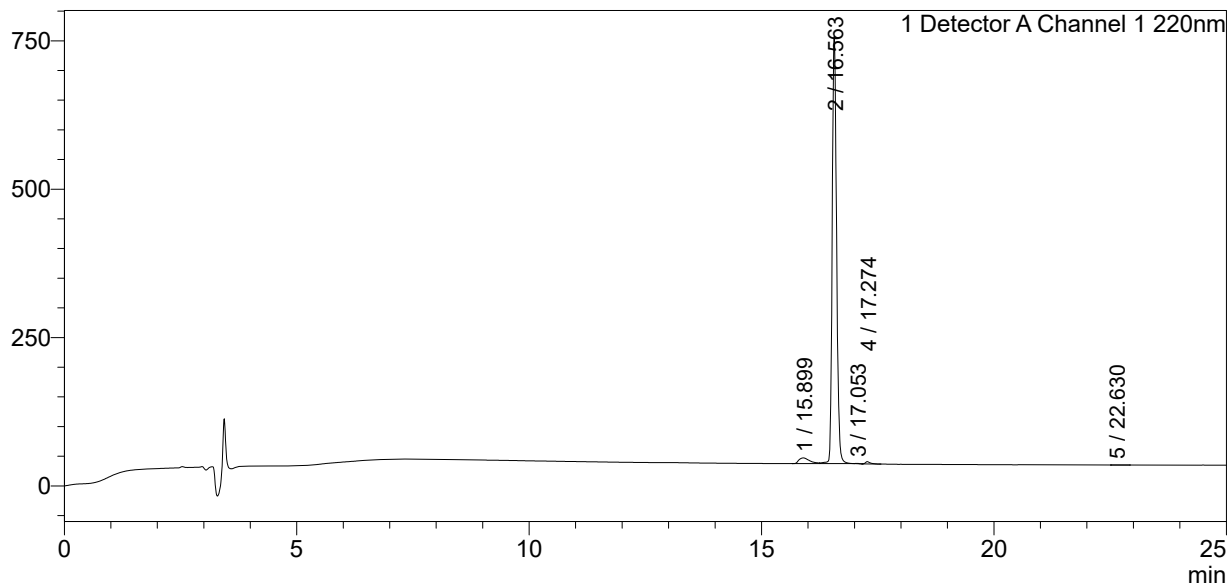

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.899	152560	9561	3.145
2	16.563	4664884	720264	96.162
3	17.053	2671	587	0.055
4	17.274	27887	3887	0.575
5	22.630	3052	400	0.063
Total		4851054	734699	100.000