

Sample Name : β -Amyloid (33-40)
 Cat No.: RP20144
 Lot No.: E6033620C
 Time Processed :16:10:55
 Month-Day-Year Processed :03/31/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

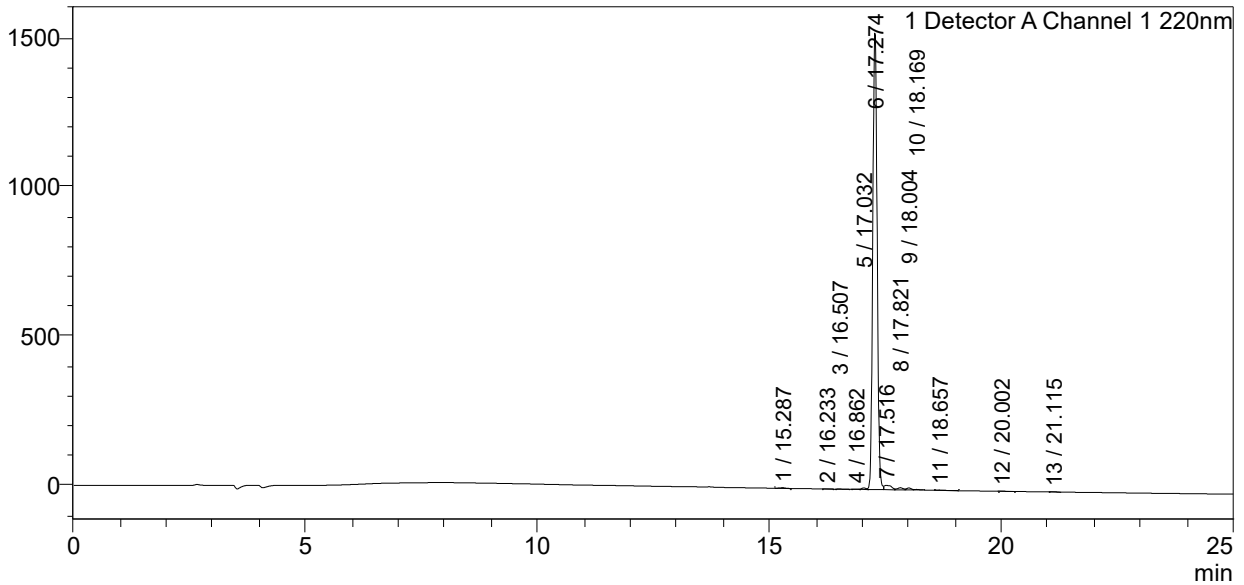

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.287	16775	2081	0.162
2	16.233	3699	509	0.036
3	16.507	4492	803	0.043
4	16.862	4573	774	0.044
5	17.032	30939	5085	0.298
6	17.274	10012385	1529844	96.545
7	17.516	164629	14403	1.587
8	17.821	55279	6942	0.533
9	18.004	47886	6596	0.462
10	18.169	13262	1788	0.128
11	18.657	11741	1056	0.113
12	20.002	2331	279	0.022
13	21.115	2736	437	0.026
Total		10370727	1570596	100.000