

Sample Name :GRGDSPC  
 Cat. No. : RP20283  
 Lot. No. : E9684419J  
 Time Processed :9:39:04  
 Month-Day-Year Processed : 10/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

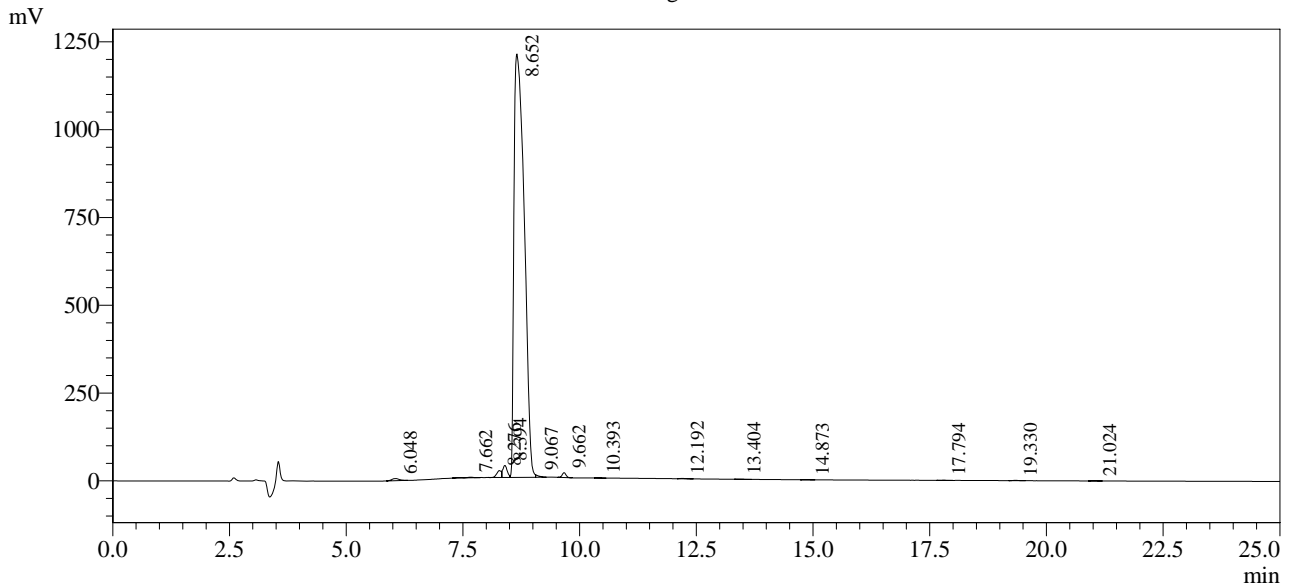

1 Det.A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.048	68757	6193	0.363
2	7.662	26428	1765	0.139
3	8.276	136200	19399	0.719
4	8.394	221416	34123	1.168
5	8.652	18363821	1205530	96.907
6	9.067	29432	6558	0.155
7	9.662	78337	13837	0.413
8	10.393	1048	128	0.006
9	12.192	8018	905	0.042
10	13.404	1866	159	0.010
11	14.873	2334	332	0.012
12	17.794	3300	452	0.017
13	19.330	7015	968	0.037
14	21.024	2027	280	0.011
Total		18949998	1290630	100.000