

Sample Name : Competence-StimulatingPeptide-12261
 Cat. No. : RP20427
 Lot. No. : PE0781711

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

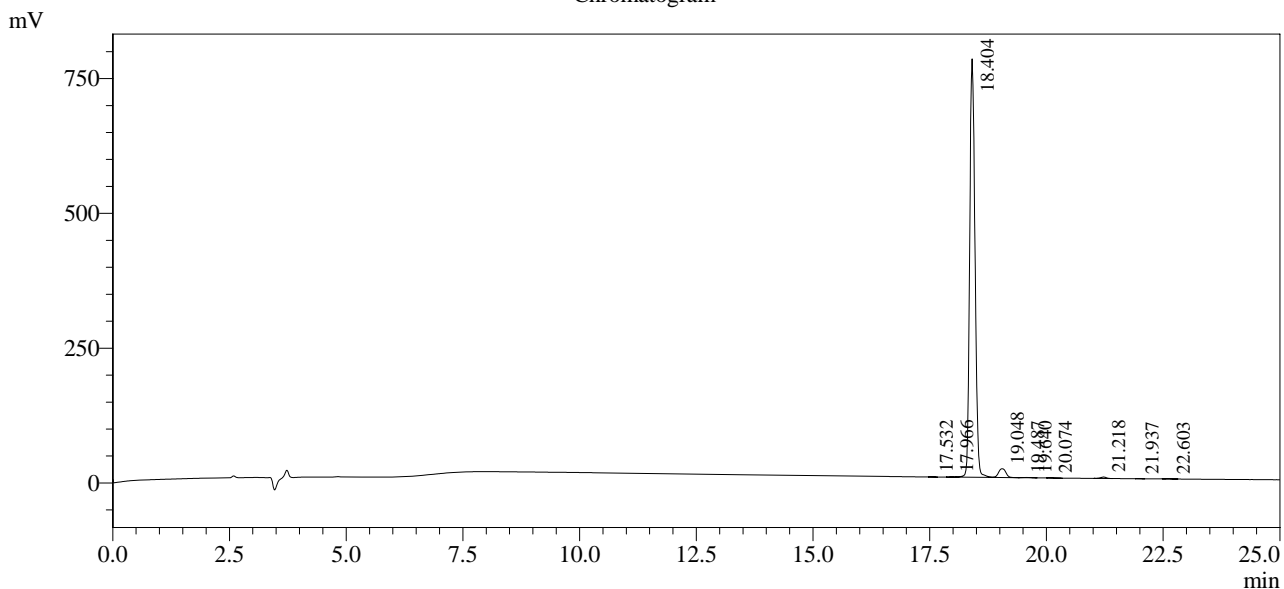

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.532	1263	199	0.020
2	17.966	2581	361	0.040
3	18.404	6165952	776032	96.594
4	19.048	178401	16229	2.795
5	19.487	1983	268	0.031
6	19.640	2484	371	0.039
7	20.074	1544	184	0.024
8	21.218	22276	2666	0.349
9	21.937	1399	203	0.022
10	22.603	5510	692	0.086
Total		6383394	797206	100.000