

Sample Name: Peptide C105Y
 Cat. No. : RP20382
 Lot. No. : E3301121C
 Time Processed: 8:05:28
 Month-Day-Year Processed :04/04/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

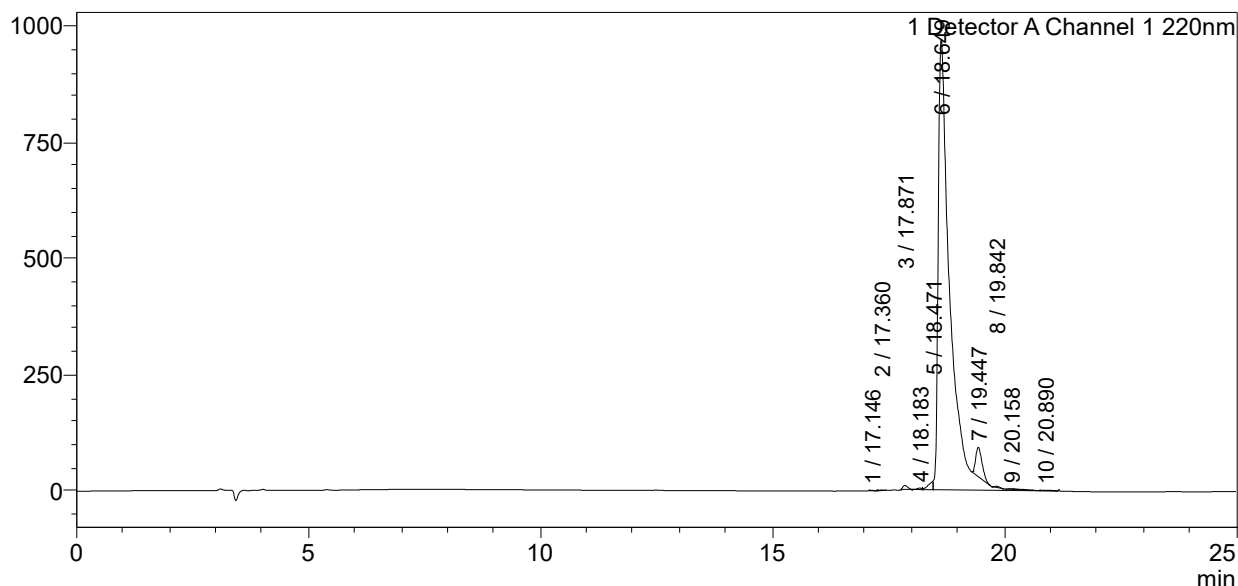

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.146	3585	767	0.020
2	17.360	8110	1371	0.045
3	17.871	58233	8253	0.325
4	18.183	24491	3001	0.137
5	18.471	126875	18062	0.708
6	18.649	17053970	967923	95.110
7	19.447	601825	63066	3.356
8	19.842	15571	2317	0.087
9	20.158	22355	965	0.125
10	20.890	15725	1150	0.088
Total		17930740	1066875	100.000