

Sample Name :mTRP-2(180-188)
 Cat. No. : RP20250
 Lot. No. : E2483420H
 Time Processed :6:02:22
 Month-Day-Year Processed : 08/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

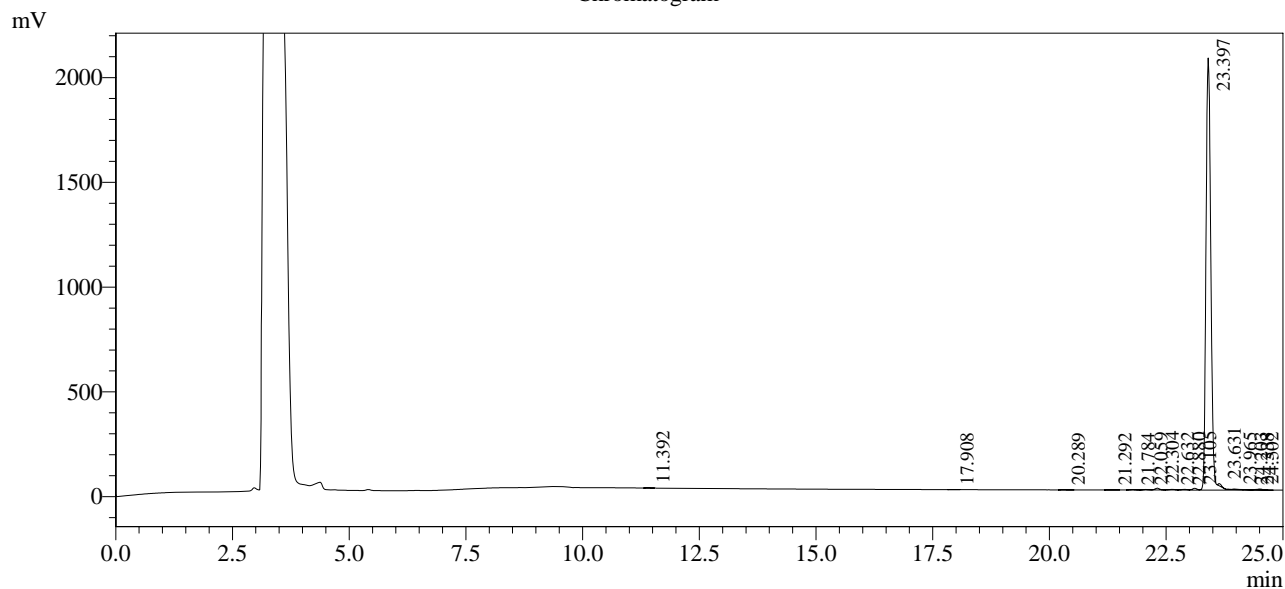

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.392	6210	1152	0.041
2	17.908	1616	301	0.011
3	20.289	2654	382	0.017
4	21.292	3185	418	0.021
5	21.784	13574	1482	0.089
6	22.059	18863	2300	0.123
7	22.304	62550	8913	0.408
8	22.632	28112	3126	0.184
9	22.880	29954	3104	0.196
10	23.105	56830	8313	0.371
11	23.397	14991347	2062269	97.875
12	23.631	47506	9894	0.310
13	23.965	12640	2241	0.083
14	24.203	6972	1356	0.046
15	24.338	5052	887	0.033
16	24.502	29720	4146	0.194
Total		15316786	2110283	100.000