

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), rat
 Cat No. :RP11195
 Lot No. :E0174021D
 Time Processed :1:01:03 AM
 Month-Day-Year Processed :04/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

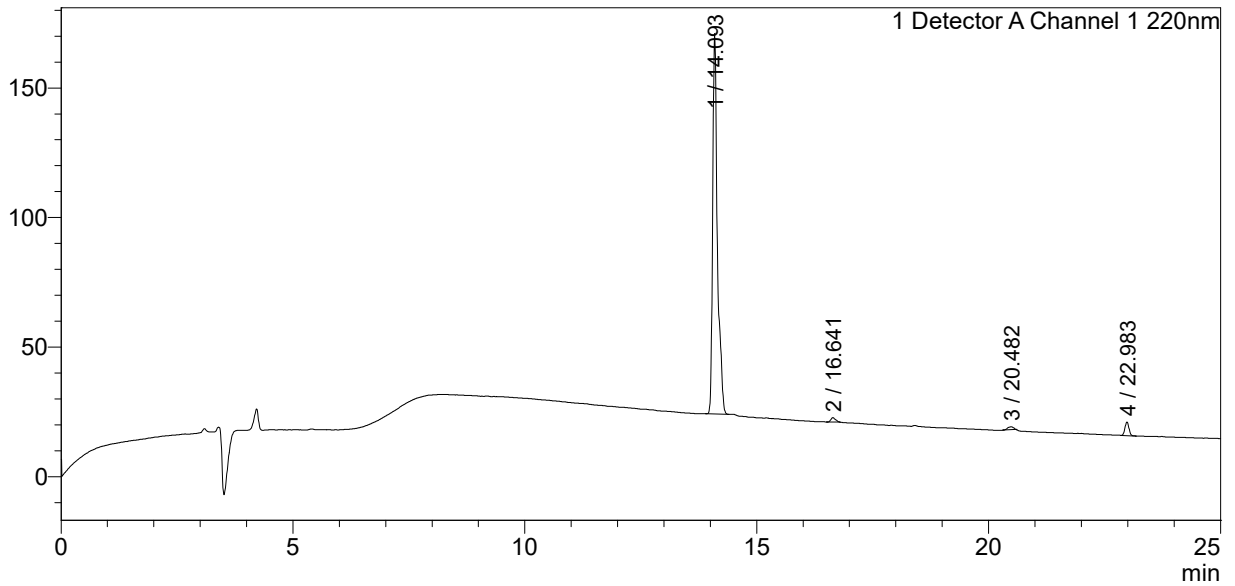

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.093	1037974	146839	95.119
2	16.641	12071	1721	1.106
3	20.482	10111	1122	0.927
4	22.983	31086	5226	2.849
Total		1091242	154908	100.000