

Sample Name : OVA Peptide (257-264)
 Cat No : RP10611
 Lot No : E3006821D
 Time Processed : 12:40:27 AM
 Month-Day-Year Processed : 04/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : GK11010011

<Chromatogram>

mV

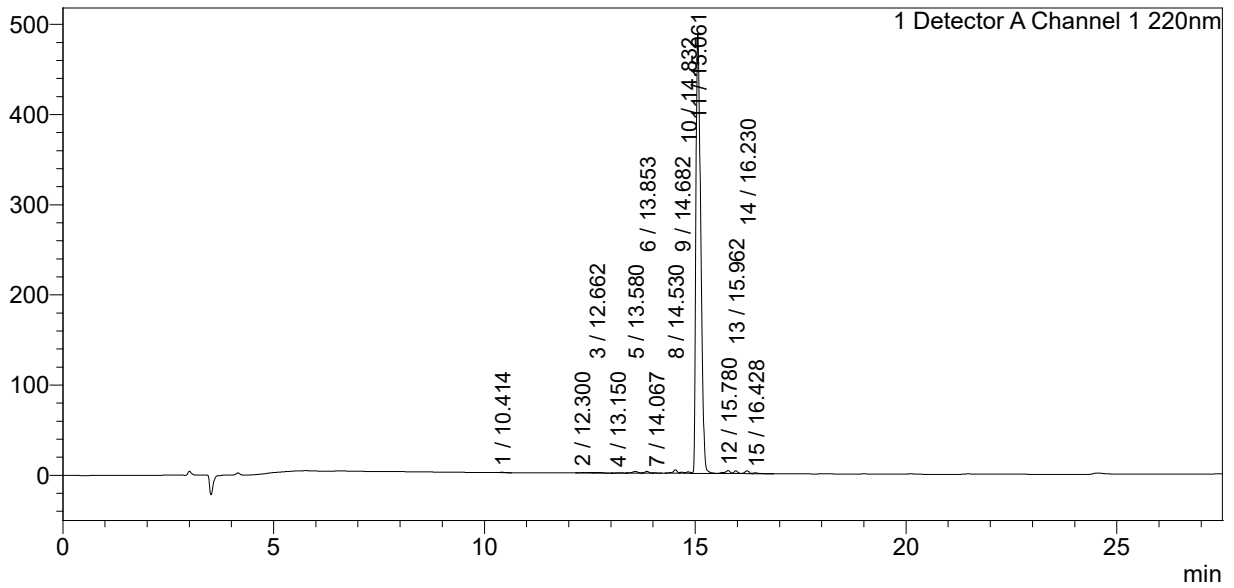

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.414	2962	442	0.073
2	12.300	7705	319	0.190
3	12.662	9217	756	0.227
4	13.150	3579	322	0.088
5	13.580	18962	1874	0.467
6	13.853	14150	2052	0.349
7	14.067	2448	388	0.060
8	14.530	27907	3764	0.688
9	14.682	6777	1258	0.167
10	14.832	11759	1594	0.290
11	15.061	3876813	485355	95.518
12	15.780	27741	3220	0.683
13	15.962	18459	3054	0.455
14	16.230	21554	3101	0.531
15	16.428	8710	1109	0.215
Total		4058743	508609	100.000