

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :PE5241901
 Time Processed :12:25:46
 Month-Day-Year Processed :01/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

mV

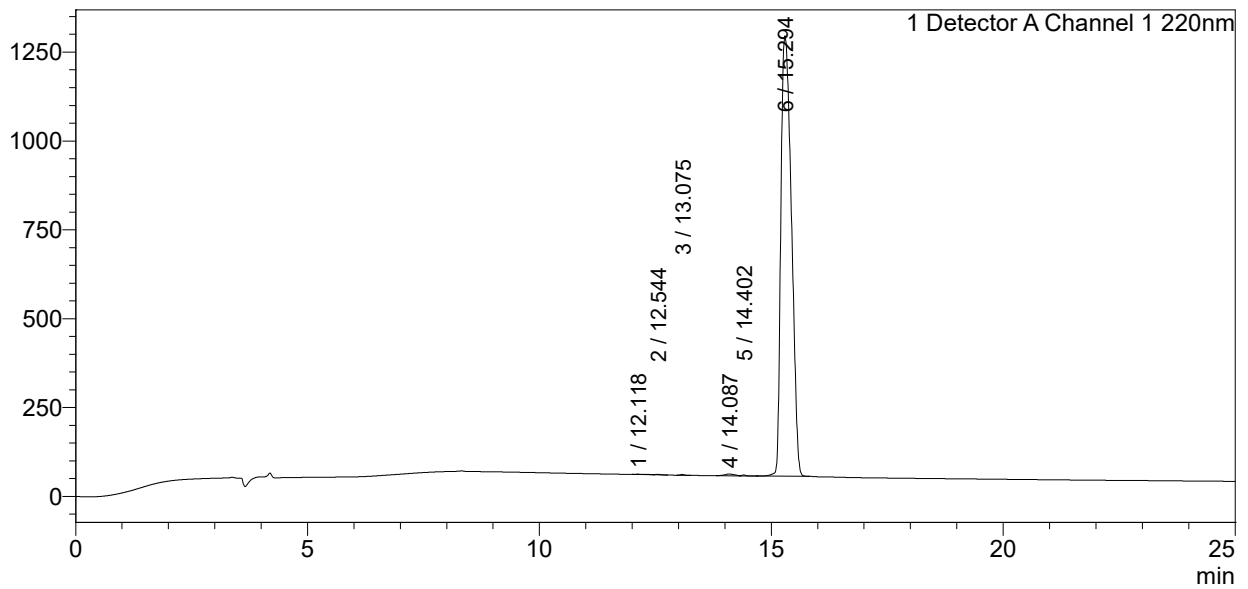

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.118	12026	972	0.061
2	12.544	7254	990	0.037
3	13.075	14274	2285	0.072
4	14.087	74553	5167	0.379
5	14.402	16697	2532	0.085
6	15.294	19571015	1239593	99.366
Total		19695819	1251539	100.000