

Sample Name :LSKL, Inhibitor of Thrombospondin (TSP-1)
 Cat No. :RP19990
 Lot No. :E9411720B
 Time Processed :9:11:30
 Month-Day-Year Processed :02/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

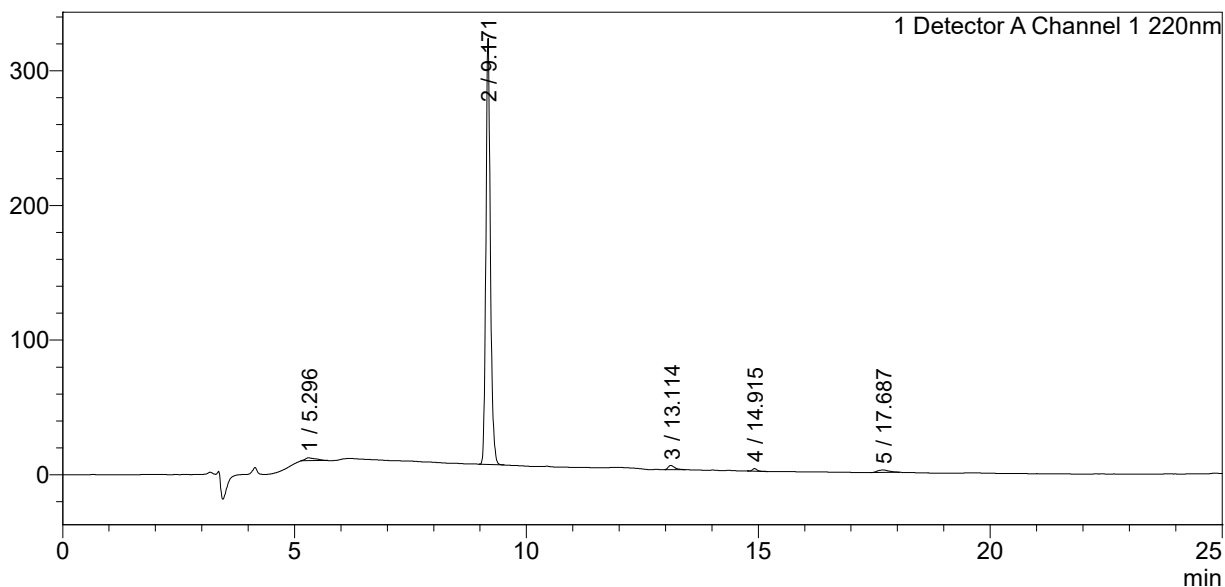

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.296	35045	2159	1.562
2	9.171	2132612	316646	95.061
3	13.114	30367	3161	1.354
4	14.915	14108	1990	0.629
5	17.687	31277	1830	1.394
Total		2243409	325786	100.000