

Sample Name : Glucagon (19-29), human
 Cat No. : RP10770
 Lot No. : E4754919I
 Time Processed : 3:11:40
 Month-Day-Year Processed : 09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010507

<Chromatogram>

mV

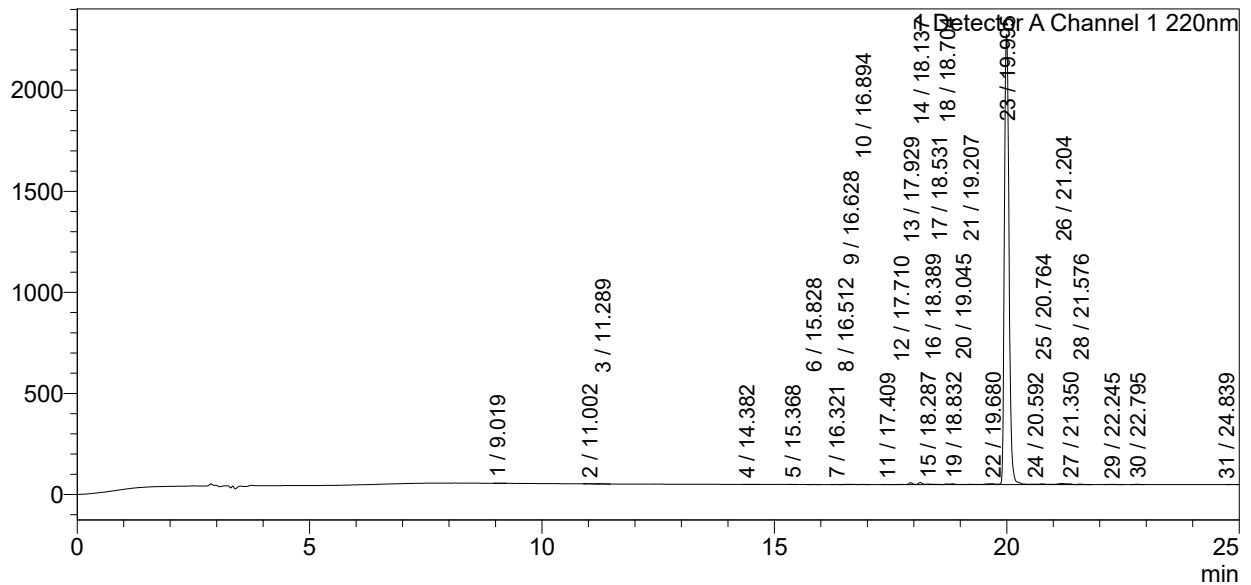

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.019	1977	238	0.012
2	11.002	5132	751	0.032
3	11.289	3980	640	0.025
4	14.382	2702	213	0.017
5	15.368	1220	335	0.008
6	15.828	2750	417	0.017
7	16.321	3715	596	0.023
8	16.512	5127	866	0.032
9	16.628	11636	1387	0.073
10	16.894	7735	875	0.049
11	17.409	3217	488	0.020
12	17.710	11100	1146	0.070
13	17.929	51169	8951	0.323
14	18.137	58550	10186	0.369
15	18.287	11383	2207	0.072

Peak#	Ret. Time	Area	Height	Area%
16	18.389	14344	2258	0.090
17	18.531	7171	1312	0.045
18	18.704	16508	2977	0.104
19	18.832	26580	3996	0.168
20	19.045	8308	1123	0.052
21	19.207	10563	1445	0.067
22	19.680	63577	4320	0.401
23	19.995	15408698	2226741	97.144
24	20.592	2362	437	0.015
25	20.764	16055	2586	0.101
26	21.204	44788	4272	0.282
27	21.350	20570	3098	0.130
28	21.576	13220	1937	0.083
29	22.245	12193	1024	0.077
30	22.795	9398	1464	0.059
31	24.839	6059	683	0.038
Total		15861787	2288969	100.000