

Sample Name : CEF7, Influenza Virus NP (380-388)
 Cat No: RP20419
 Lot No : E7321521C
 Time Processed : 11:34:03
 Month-Day-Year Processed : 03/22/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
25.00	Pumps	B.Conc	60
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	0
40.00	Pumps	B.Conc	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

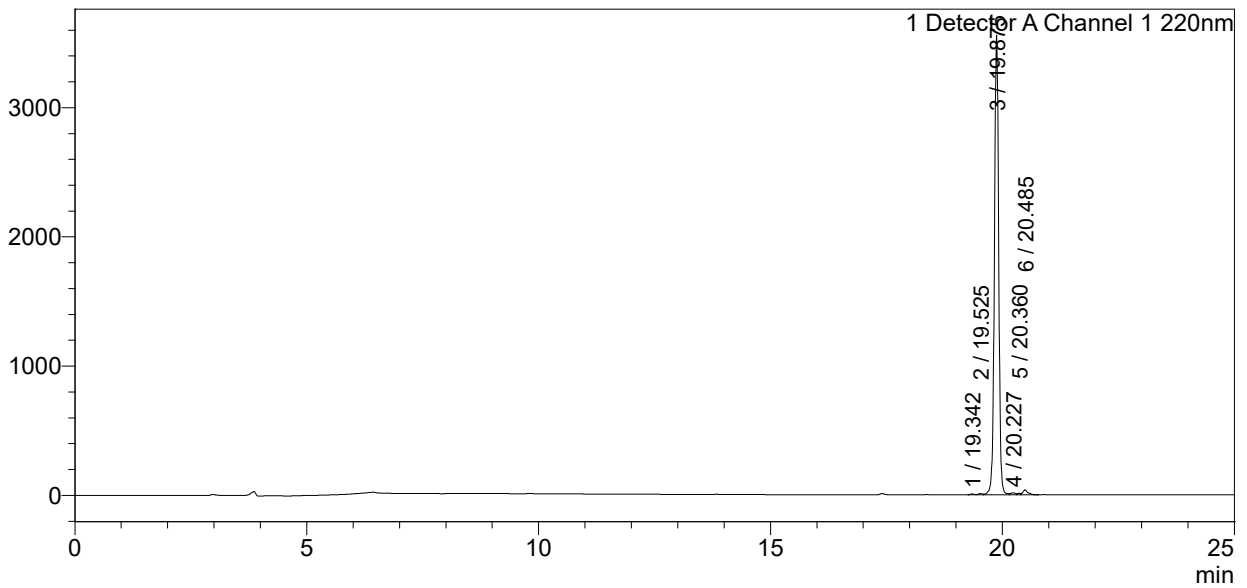

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	19.342	35980	5915	0.153
2	19.525	57784	8972	0.245
3	19.875	23044224	3558143	97.677
4	20.227	111237	15912	0.471
5	20.360	56348	11316	0.239
6	20.485	286627	38801	1.215
Total		23592200	3639058	100.000