

Sample Name:Glucagon (19-29), human
 Cat No:RP10770
 Lot No:E9907121F
 Time Processed :1:52:54 AM
 Month-Day-Year Processed :06/11/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

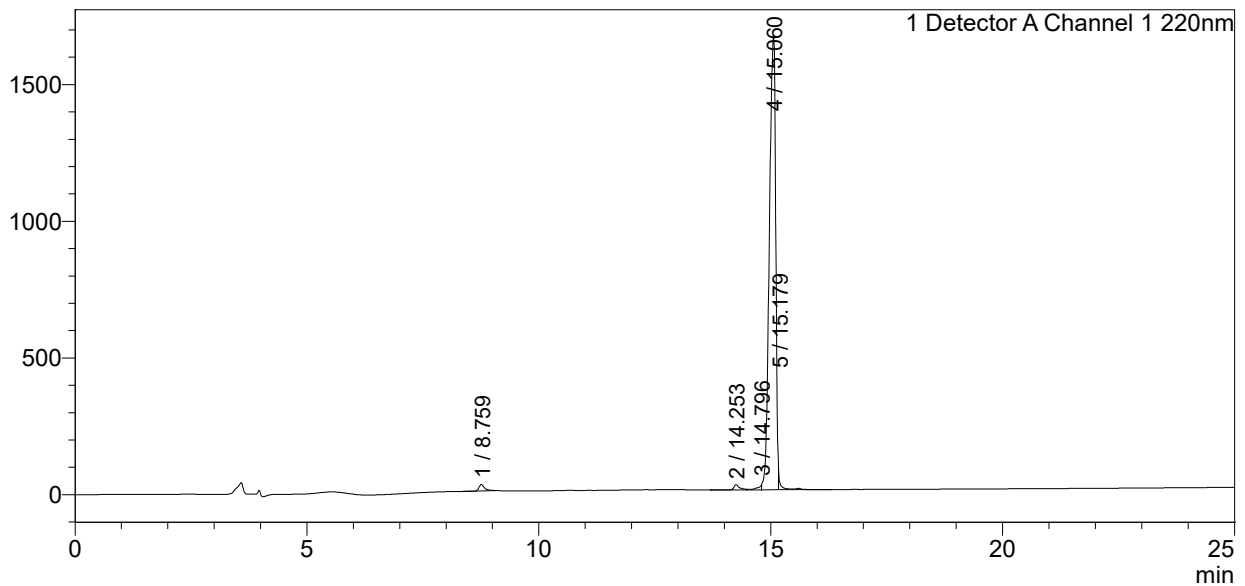

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.759	186123	23259	1.141
2	14.253	152809	18972	0.937
3	14.796	107084	16130	0.656
4	15.060	15635016	1661543	95.836
5	15.179	233309	58096	1.430
Total		16314341	1778000	100.000