


Mass Spectrum

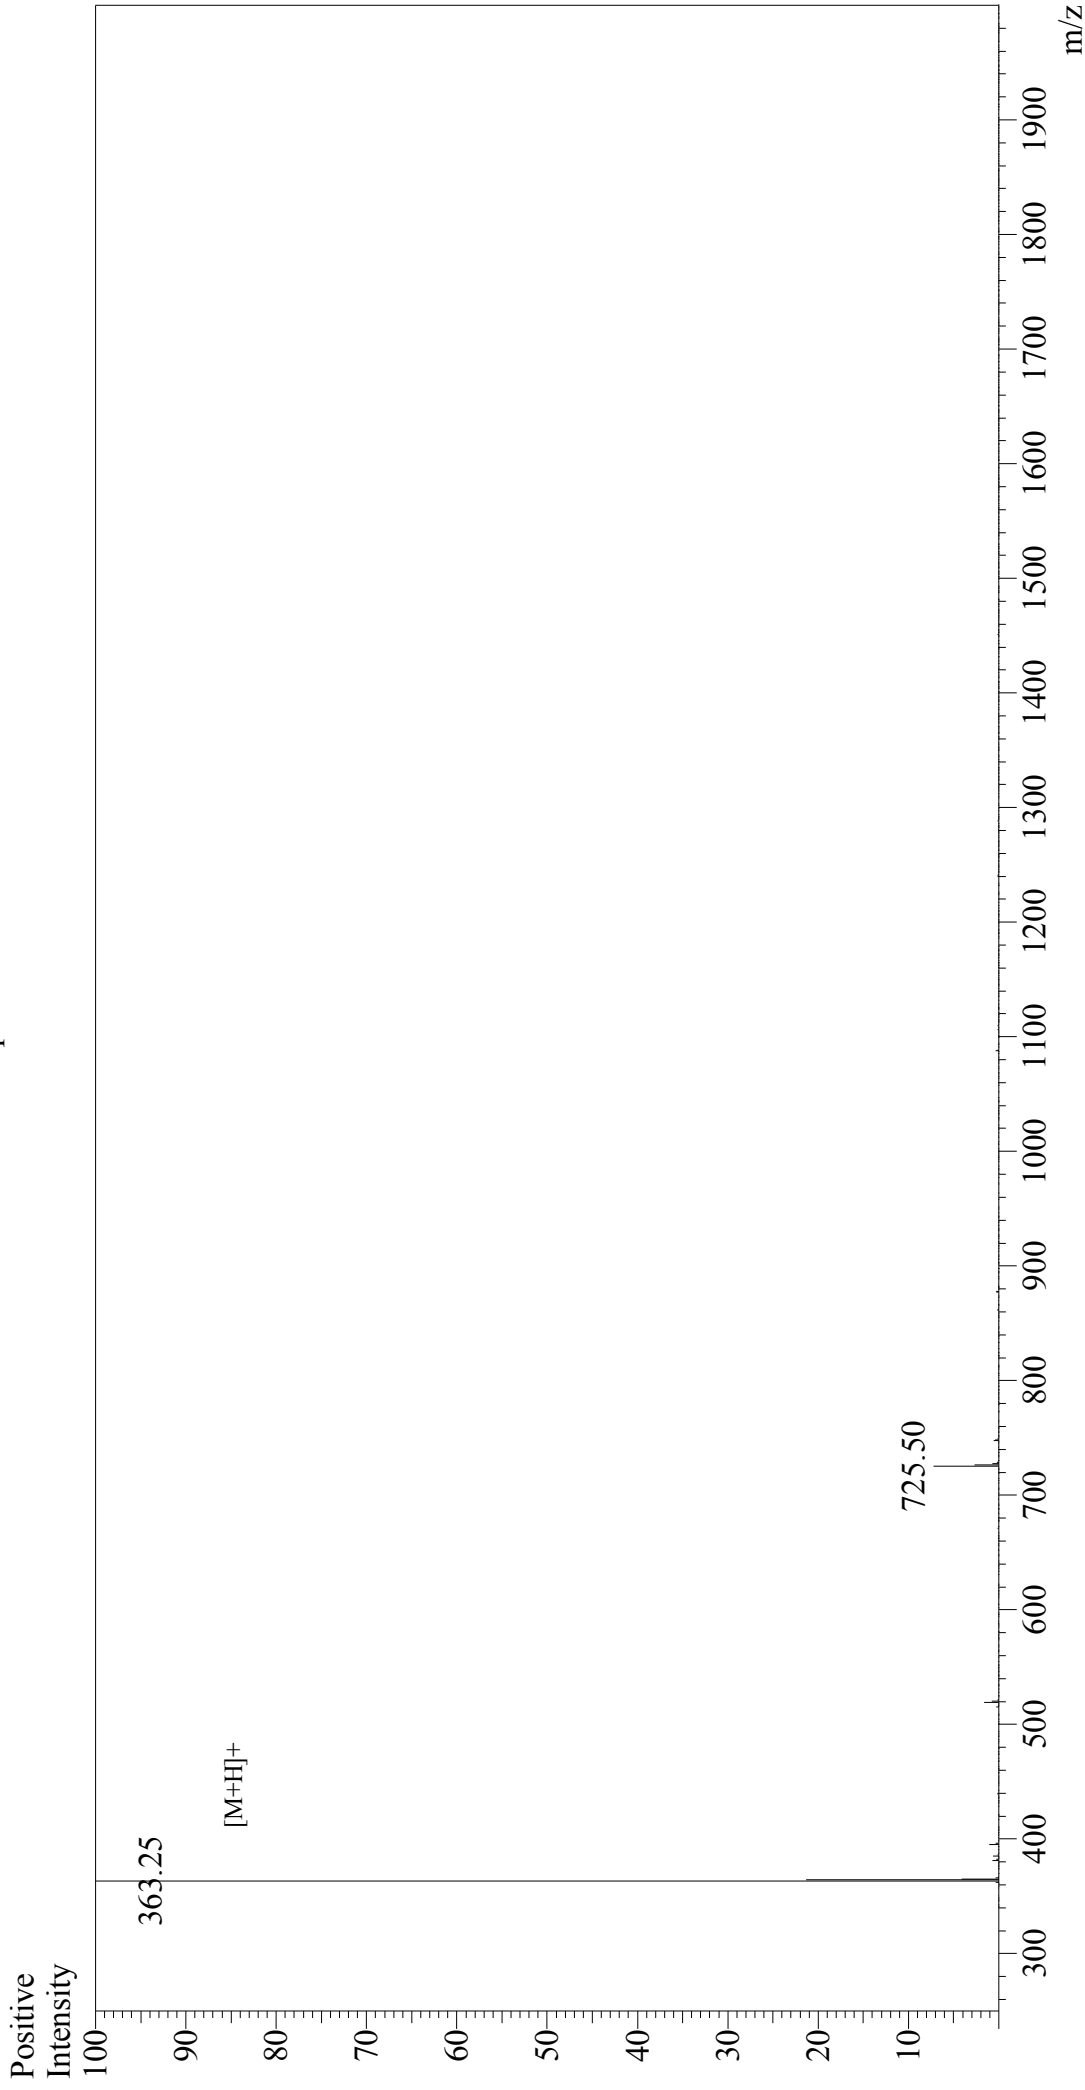

Sample Information

Acquired by : Gary
Month-Day Processed : 07/08/18
Time Processed : 10:39:16
Injection Volume : 0.2
Sample Name : Thyrotropin-Releasing Hormone (TRH)
Cat. No. : RP10112
Lot. No. : PE0031806
Theoretical MW : 362.38
Observed MW : 362.25

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH