

Sample Name : Influenza A NP(366-374) Strain A/PR/8/35
 Cat. No. : RP20267
 Lot. No. : E3879020G
 Time Processed : 7:42:38
 Month-Day-Year Processed : 07/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

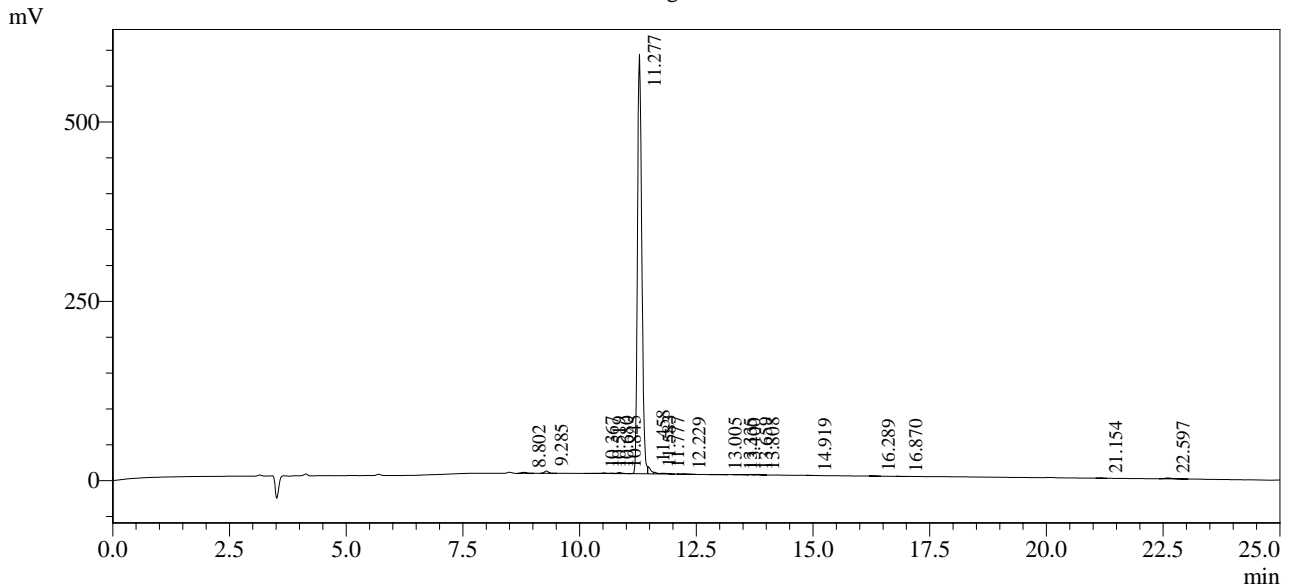

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.802	8891	1355	0.226
2	9.285	19861	3241	0.505
3	10.367	2287	224	0.058
4	10.519	5819	838	0.148
5	10.680	3723	598	0.095
6	10.845	9354	1417	0.238
7	11.277	3780319	584782	96.173
8	11.458	42198	10054	1.074
9	11.583	11379	2433	0.289
10	11.777	10657	986	0.271
11	12.229	4058	390	0.103
12	13.005	2123	220	0.054
13	13.335	1048	208	0.027
14	13.400	1257	215	0.032
15	13.659	2167	413	0.055
16	13.808	4173	703	0.106
17	14.919	1221	195	0.031
18	16.289	1759	237	0.045
19	16.870	1015	157	0.026
20	21.154	2273	385	0.058
21	22.597	15161	1266	0.386
Total		3930743	610319	100.000