

Sample Name :Osteogenic Growth Peptide,OGP

Cat. No. : RP20311

Lot. No. : PE6221808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

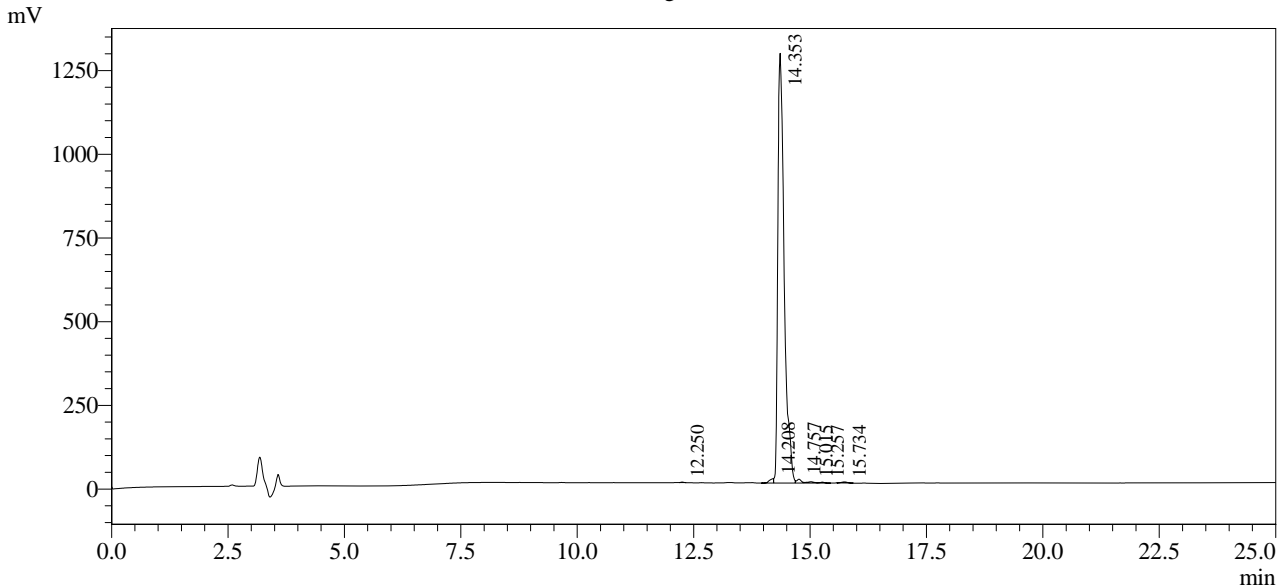

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.250	6496	1547	0.052
2	14.208	80471	13548	0.644
3	14.353	12244192	1283286	97.926
4	14.757	78968	11655	0.632
5	15.015	44793	4135	0.358
6	15.257	20420	2883	0.163
7	15.734	28120	3162	0.225
Total		12503460	1320216	100.000