

Sample Name :p5 Ligand for Dnak and and D naJ
 Cat. No. : RP20327
 Lot. No. : PE0271706

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

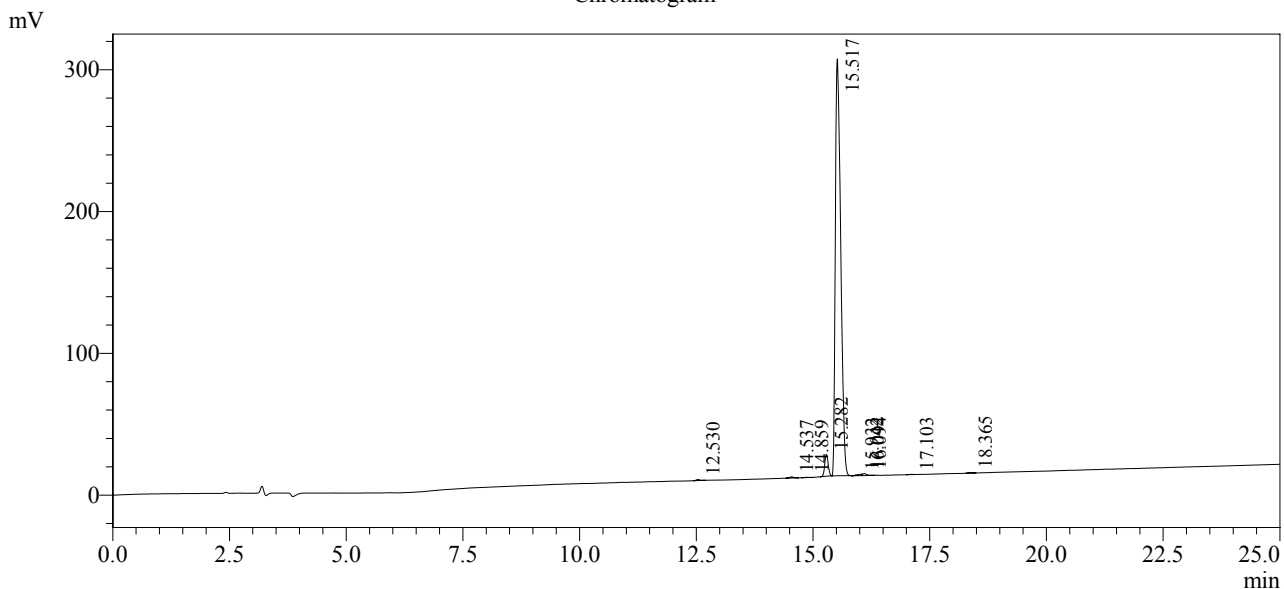

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.530	4307	774	0.175
2	14.537	4603	713	0.187
3	14.859	1345	222	0.055
4	15.282	79285	15434	3.220
5	15.517	2354365	294015	95.605
6	15.932	2864	660	0.116
7	16.042	4961	1085	0.201
8	16.094	8126	1358	0.330
9	17.103	1166	199	0.047
10	18.365	1583	276	0.064
Total		2462606	314735	100.000