

Sample Name : C-Peptide (3-33), human  
 Cat. No. : RP11116  
 Lot. No. : PE3301705

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

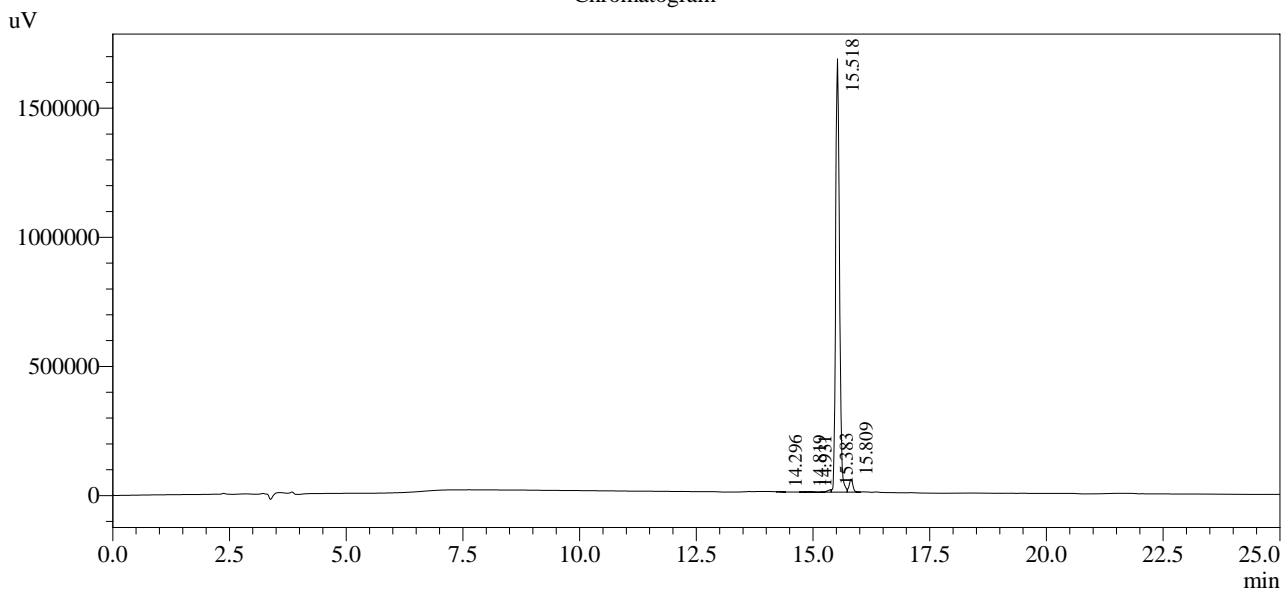

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.296	6400	1265	0.065
2	14.819	7054	1133	0.071
3	14.931	11791	1300	0.119
4	15.383	53329	9620	0.538
5	15.518	9561696	1678083	96.431
6	15.809	275290	49904	2.776
Total		9915561	1741305	100.000